

Y Value Scales Centered on Mean Values

Step Between Measured Pole Tips = 5

Regression Line Through Points = -----

Dimensions in mm



LCLS II - SXR Undulator

Nominal Gap = 14 Nominal Taper = 0.000
 Gap Reading = 14.0000 US Encoder = 14.0000 DS Encoder = 14.0000


05-APR-2019

S/N = 002

D/S = 0001

Run = 12

Gap Between Opposing Pole Tips

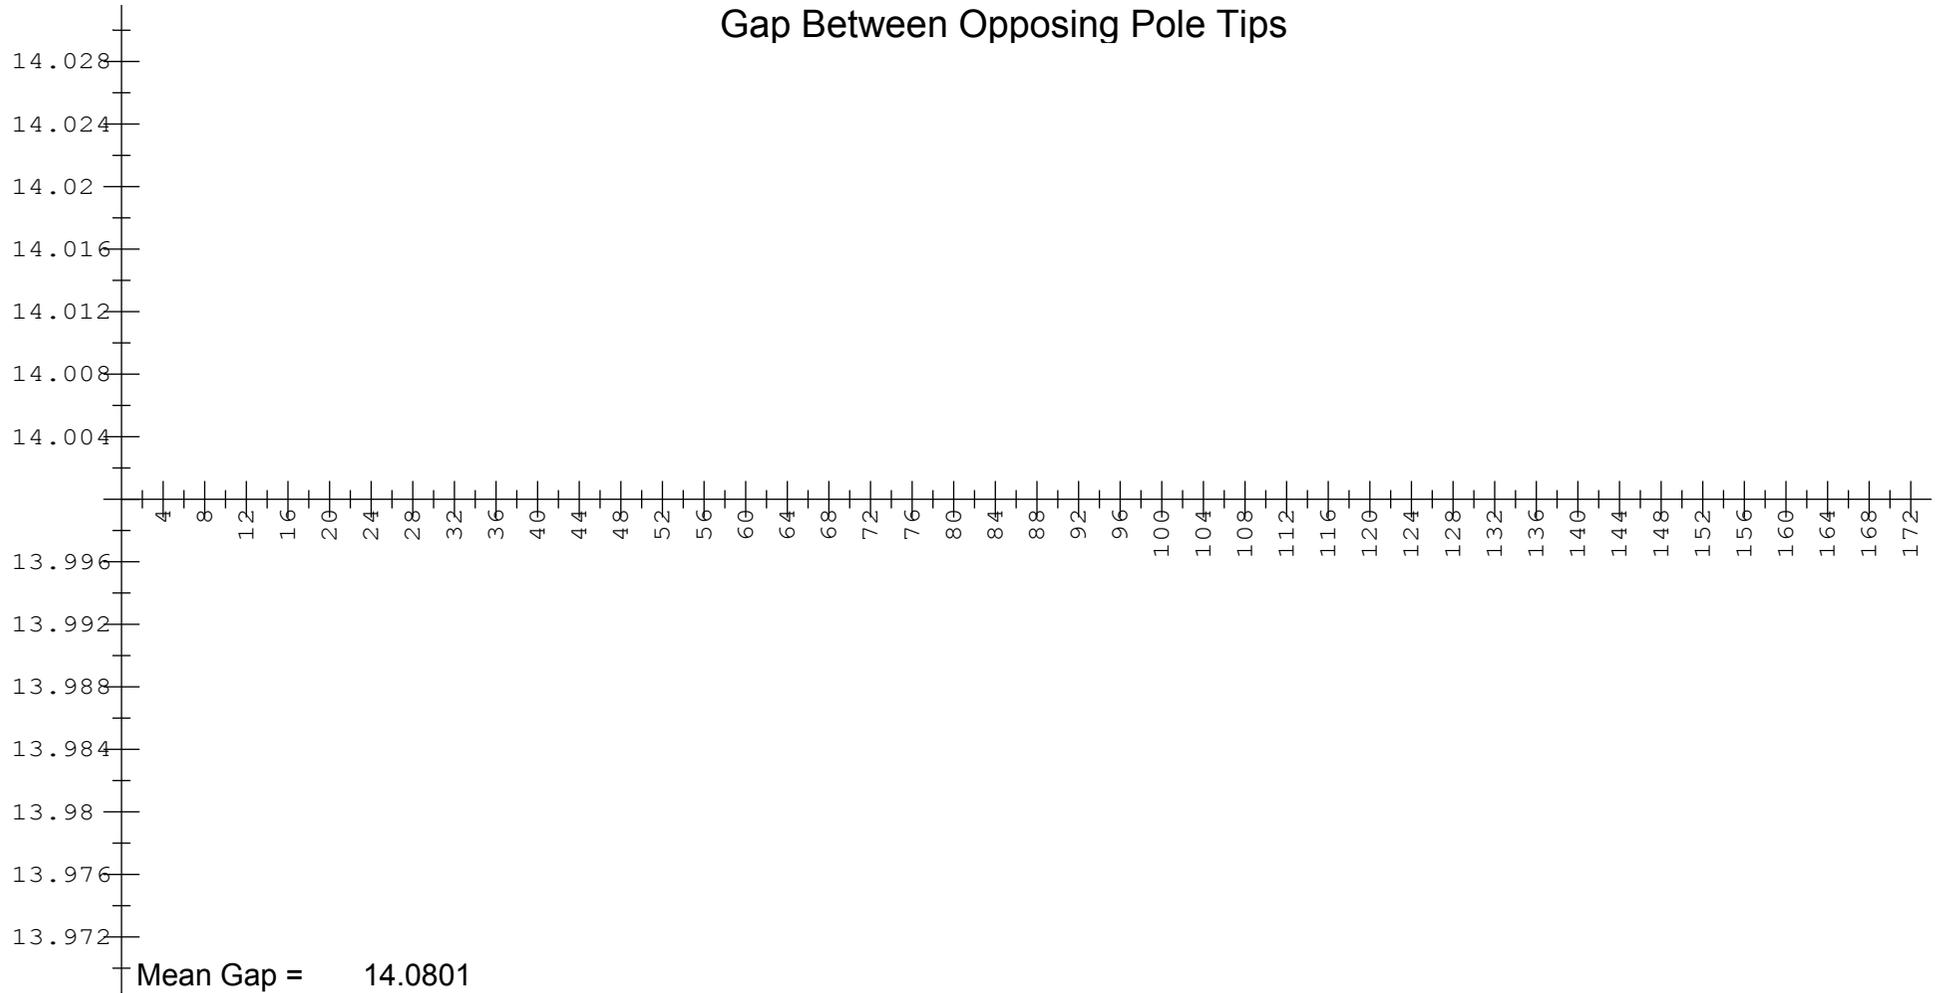

Step Between Measured Pole Tips = 5

Dimensions in mm




LCLS II - SXR Undulator

Nominal Gap = 14 Nominal Taper = 0.000
 Gap Reading = 14.0000 US Encoder = 14.0000 DS Encoder = 14.0000

05-APR-2019
 S/N = 002
 D/S = 0001
 Run = 12

Symmetry Point Between Pole Tips

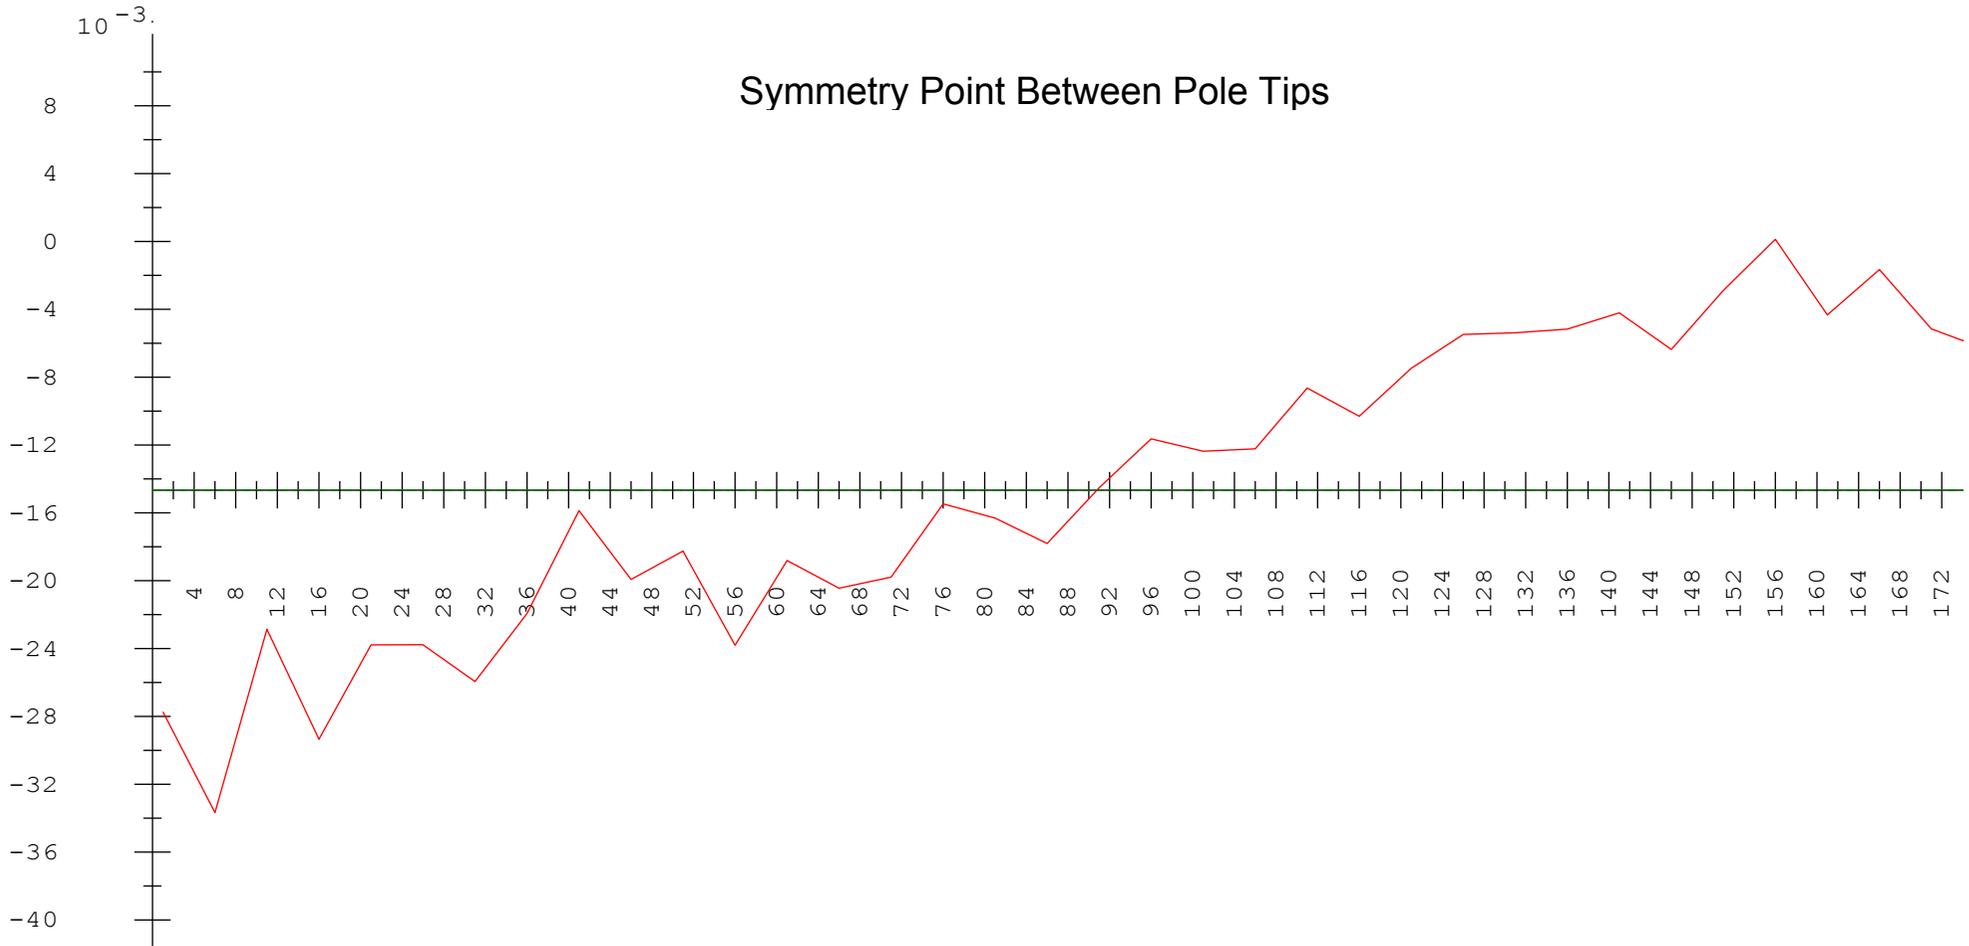

Mean Symmetry Value = -0.0147

Step Between Measured Pole Tips = 5

Dimensions in mm



LCLS II - SXR Undulator

Nominal Gap = 14 Nominal Taper = 0.000
 Gap Reading = 14.0000 US Encoder = 14.0000 DS Encoder = 14.0000

05-APR-2019
 S/N = 002
 D/S = 0001
 Run = 12

Top and Bottom Jaw Regression Line Intersect Points

Jaw	First Pole (Pole 1)	US Actuator (Pole 39)	DS Actuator (Pole 135)	Last Pole (Pole 174)
Top	7.0092	7.0164	7.0347	7.0421
Bottom	-7.0661	-7.0611	-7.0486	-7.0435
Gap	14.0753			14.0856
Taper				0.0103

Summary of Mean Values

Top Jaw Poles	Btm. Jaw Poles	Gap Values	Sym. Pt. Values
7.0254	-7.0547	14.0801	-0.0147

Additional Calculated Values

Bottom Pole #1 Z Value	980.303
Top Jaw Pitch (mrad)	0.010
Bottom Jaw Pitch(mrad)	0.007
Minimum Effective Gap	14.029
Reference Block Gap	6.810

Dimensions in mm



LCLS II - SXR Undulator

Nominal Gap = 14 Nominal Taper = 0.000
 Gap Reading = 14.0000 US Encoder = 14.0000 DS Encoder = 14.0000

05-APR-2019
 S/N = 002
 D/S= 0001
 Run= 12