

Y Value Scales Centered on Mean Values
 Step Between Measured Pole Tips = 1

Regression Line Through Points =
 Dimensions in mm



LCLS II - SXR Undulator

Nominal Gap = 10

Gap Reading = 10.0000 US Encoder = 10.0000 DS Encoder = 10.0000


07-MAR-2018

S/N = 007

D/S = 0001

Run = 3

Gap Between Opposing Pole Tips

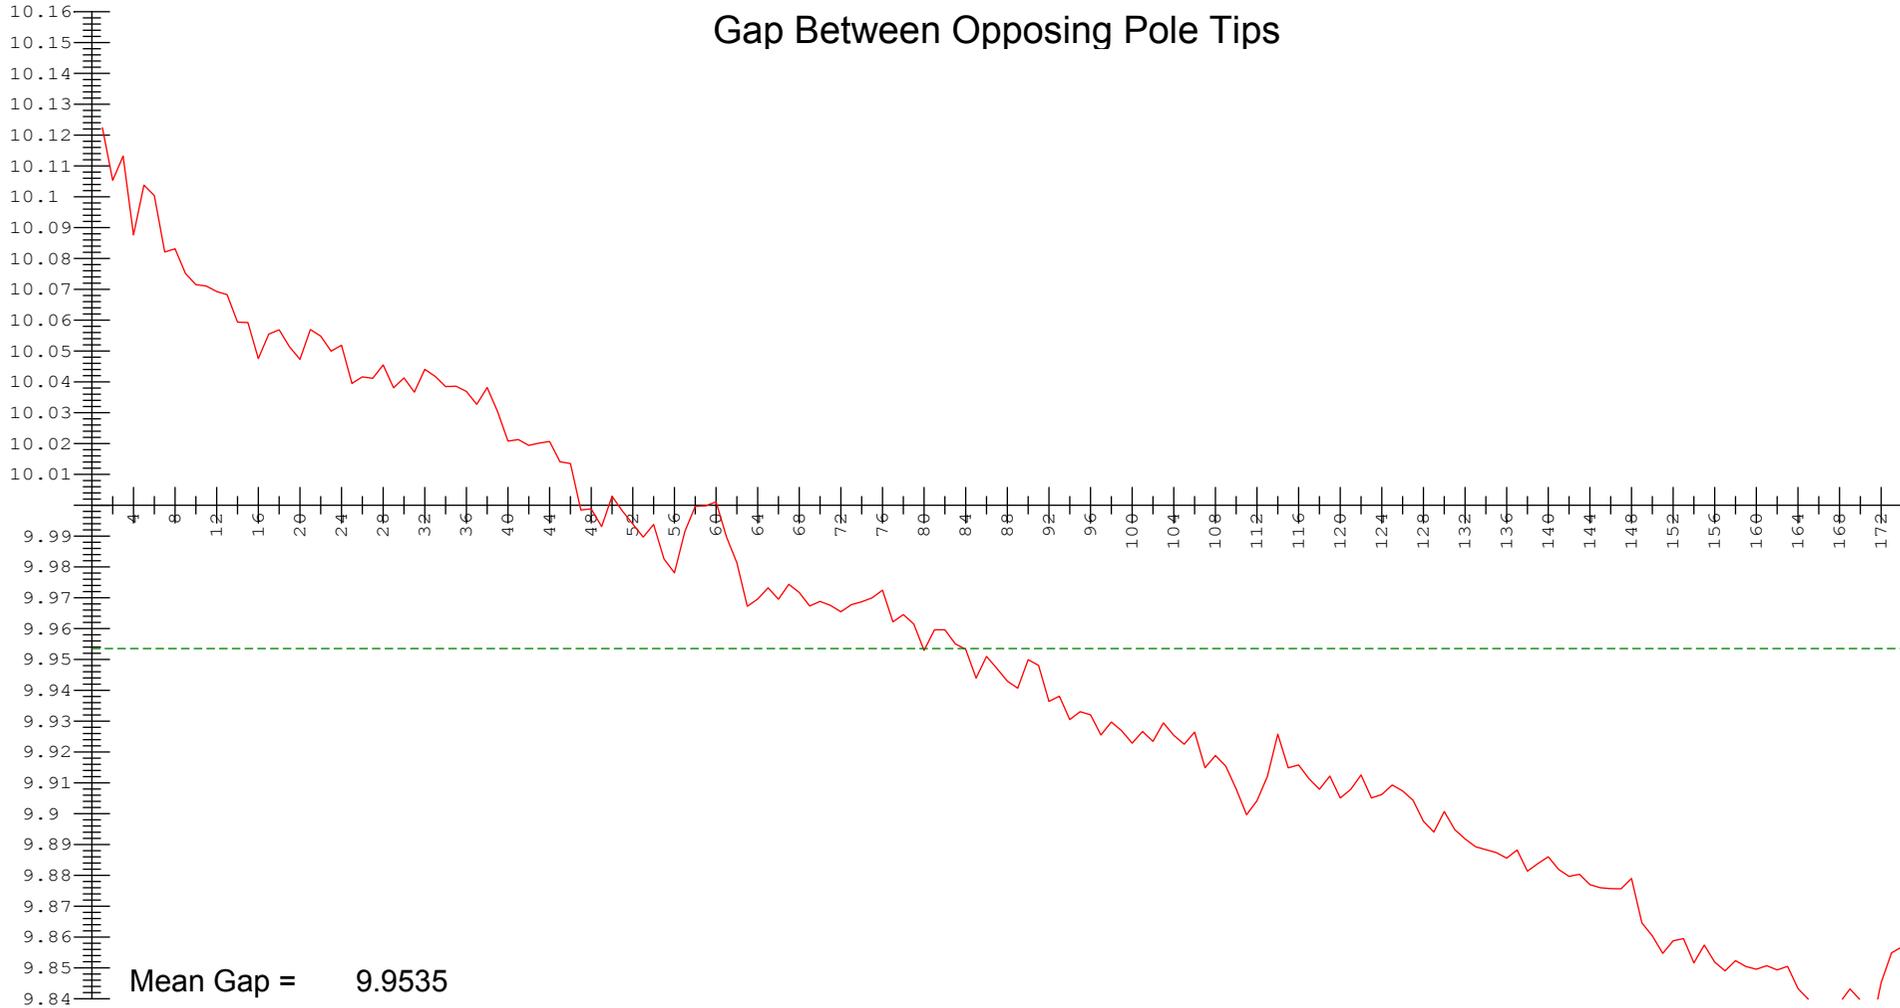

Step Between Measured Pole Tips = 1

Dimensions in mm



LCLS II - SXR Undulator

Nominal Gap = 10

Gap Reading = 10.0000 US Encoder = 10.0000 DS Encoder = 10.0000


07-MAR-2018

S/N = 007

D/S = 0001

Run = 3

Symmetry Point Between Pole Tips

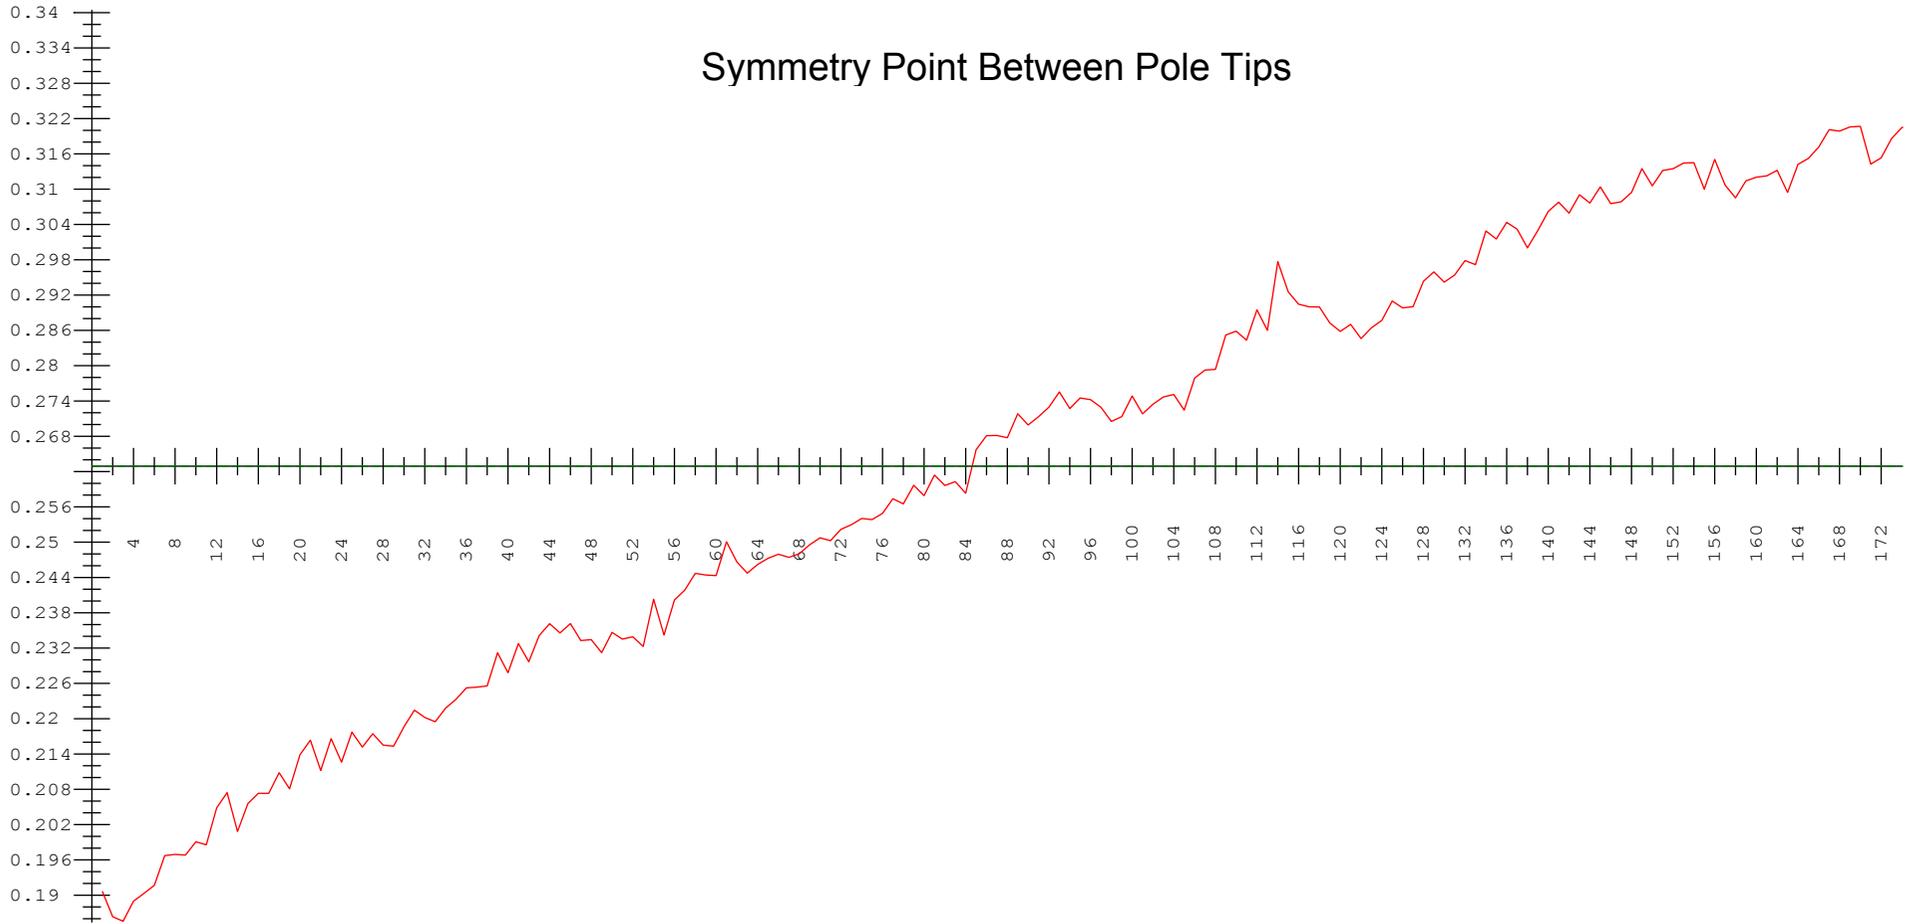

Mean Symmetry Value = 0.2629

Step Between Measured Pole Tips = 1

Dimensions in mm



LCLS II - SXR Undulator

Nominal Gap = 10

Gap Reading = 10.0000 US Encoder = 10.0000 DS Encoder = 10.0000

07-MAR-2018

S/N = 007

D/S = 0001

Run = 3

Top and Bottom Jaw Regression Line Intersect Points

Jaw	First Pole (Pole 1)	US Actuator (Pole 39)	DS Actuator (Pole 135)	Last Pole (Pole 174)
Top	5.2374	5.2384	5.2409	5.2419
Bottom	-4.8429	-4.7862	-4.6430	-4.5848
Gap	10.0803			9.8267
Taper				-0.2536

Summary of Mean Values

Top Jaw Poles	Btm. Jaw Poles	Gap Values	Sym. Pt. Values
5.2397	-4.7138	9.9535	0.2629

Additional Calculated Values

Bottom Pole #1 Z Value	979.176
Top Jaw Pitch (mrad)	0.001
Bottom Jaw Pitch(mrad)	0.077
Minimum Effective Gap	9.819
Reference Block Gap	6.804

Dimensions in mm



LCLS II - SXR Undulator

Nominal Gap = 10

Gap Reading = 10.0000 US Encoder = 10.0000 DS Encoder = 10.0000

07-MAR-2018

S/N = 007

D/S= 0001

Run= 3