

Minimum Effective Gap = 14.973

Y Value Scales Centered on Mean Values

Step Between Measured Pole Tips = 5

Regression Line Through Points =

Dimensions in mm



LCLS II - SXR Undulator

Nominal Gap = 15 Nominal Taper = 0.000
 Gap Reading = 15.0000 US Encoder = 15.0000 DS Encoder = 15.0000


24-OCT-2018

S/N = 016

D/S = 0001

Run = 12

Gap Between Opposing Pole Tips

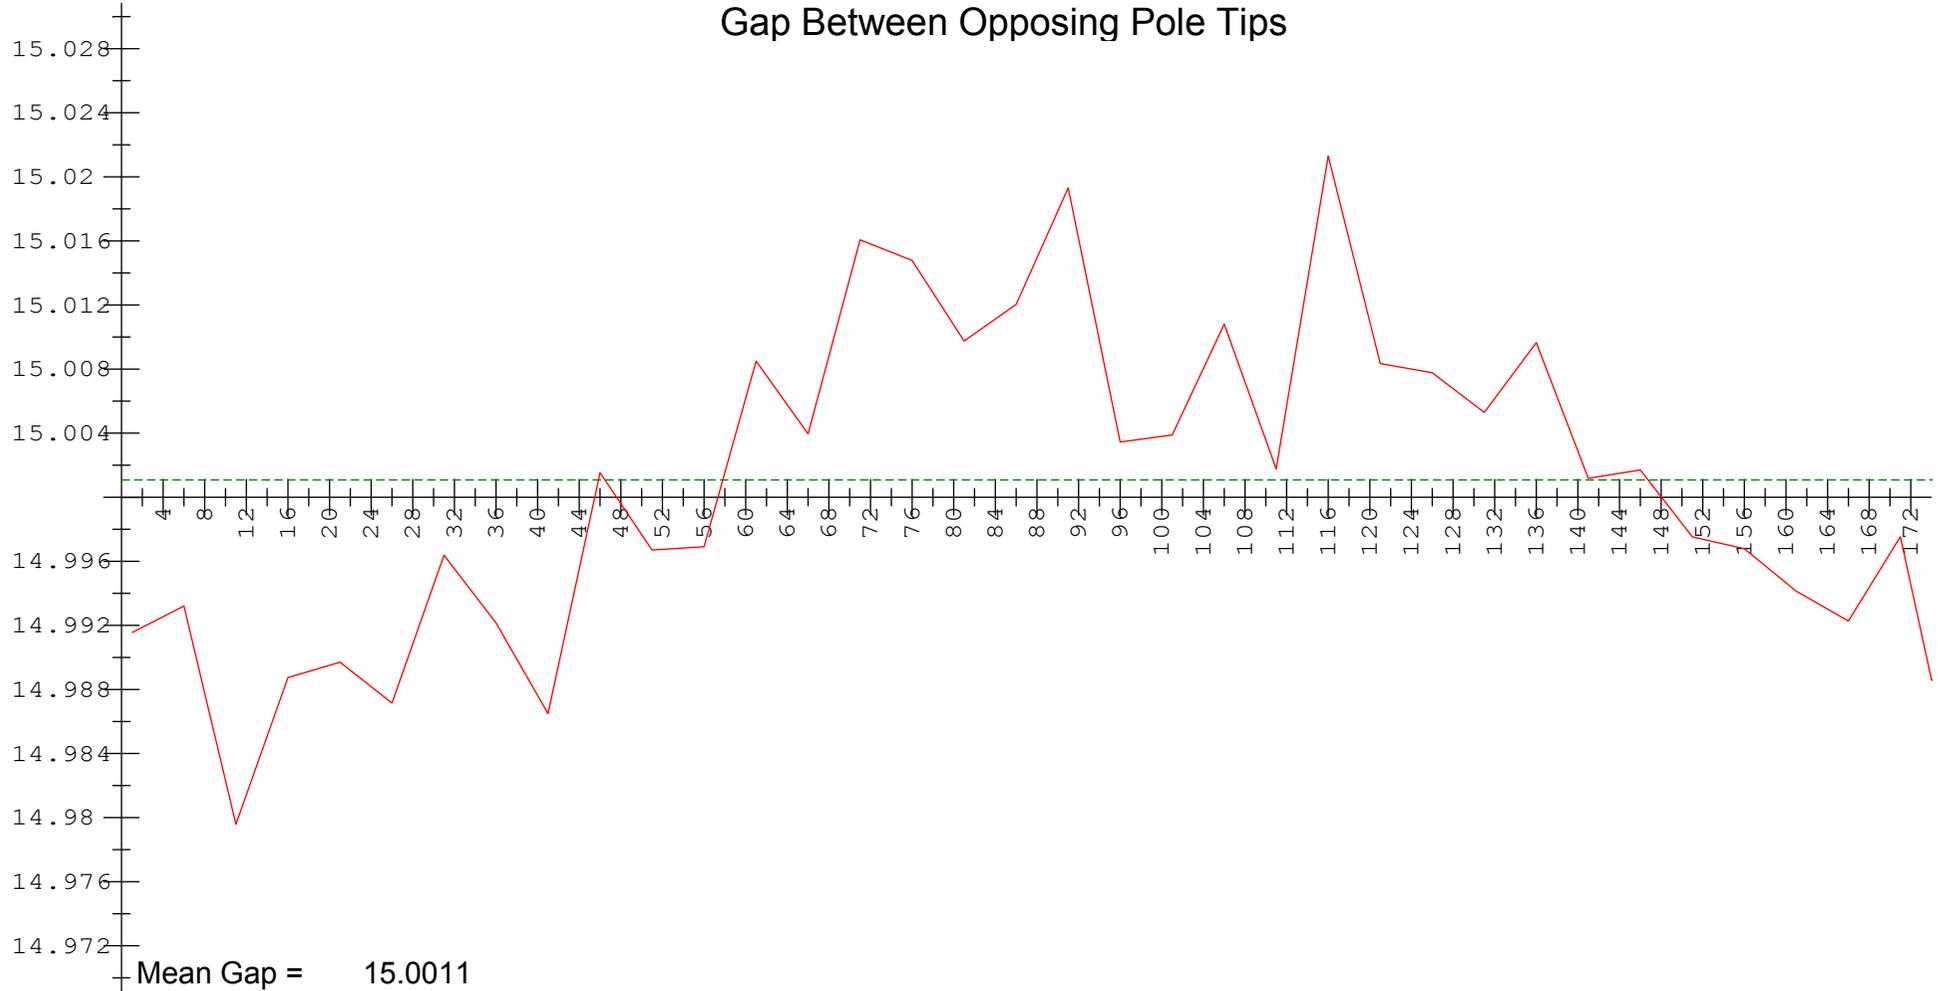

Step Between Measured Pole Tips = 5

Dimensions in mm




LCLS II - SXR Undulator

Nominal Gap = 15 Nominal Taper = 0.000
 Gap Reading = 15.0000 US Encoder = 15.0000 DS Encoder = 15.0000

24-OCT-2018
 S/N = 016
 D/S = 0001
 Run = 12

Symmetry Point Between Pole Tips

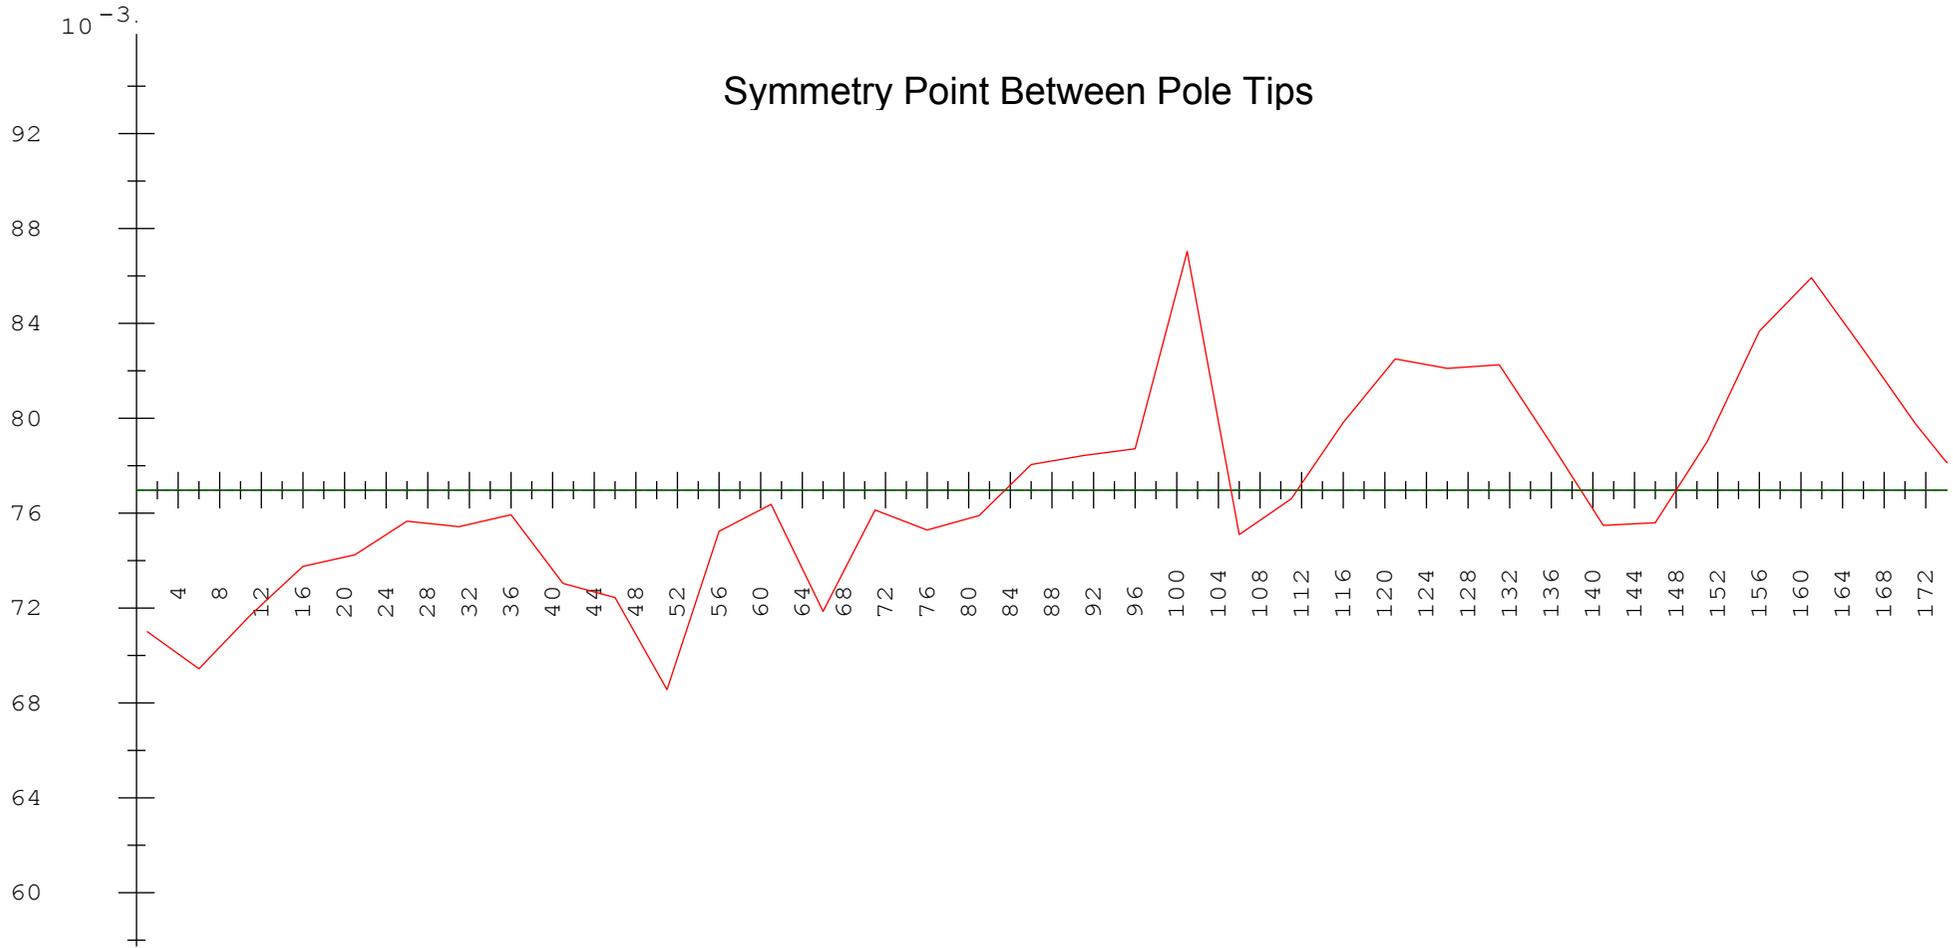

Mean Symmetry Value = 0.0770

Step Between Measured Pole Tips = 5

Dimensions in mm



LCLS II - SXR Undulator

Nominal Gap = 15 Nominal Taper = 0.000
 Gap Reading = 15.0000 US Encoder = 15.0000 DS Encoder = 15.0000

24-OCT-2018
 S/N = 016
 D/S = 0001
 Run = 12

Top and Bottom Jaw Regression Line Intersect Points

Jaw	First Pole (Pole 1)	US Actuator (Pole 39)	DS Actuator (Pole 135)	Last Pole (Pole 174)
Top	7.5696	7.5730	7.5815	7.5850
Bottom	-7.4262	-7.4250	-7.4219	-7.4206
Gap	14.9958			15.0056
Taper				0.0098

Summary of Mean Values

Top Jaw Poles	Btm. Jaw Poles	Gap Values	Sym. Pt. Values
7.5775	-7.4236	15.0011	0.0770

Additional Calculated Values

Bottom Pole #1 Z Value	979.935
Top Jaw Pitch (mrad)	0.005
Bottom Jaw Pitch(mrad)	0.002
Minimum Effective Gap	14.973
Reference Block Gap	6.809

Dimensions in mm



LCLS II - SXR Undulator

Nominal Gap = 15 Nominal Taper = 0.000
 Gap Reading = 15.0000 US Encoder = 15.0000 DS Encoder = 15.0000

24-OCT-2018
 S/N = 016
 D/S= 0001
 Run= 12