

Y Value Scales Centered on Mean Values
 Step Between Measured Pole Tips = 100

Regression Line Through Points = -----
 Dimensions in mm




LCLS II - SXR Undulator

Nominal Gap = 10 Nominal Taper = 0.000

Gap Reading = 0.0000 US Encoder = 0.0000 DS Encoder = 0.0000

30-JUL-2019
 S/N = 001
 D/S = 0007
 Run = 8

Gap Between Opposing Pole Tips

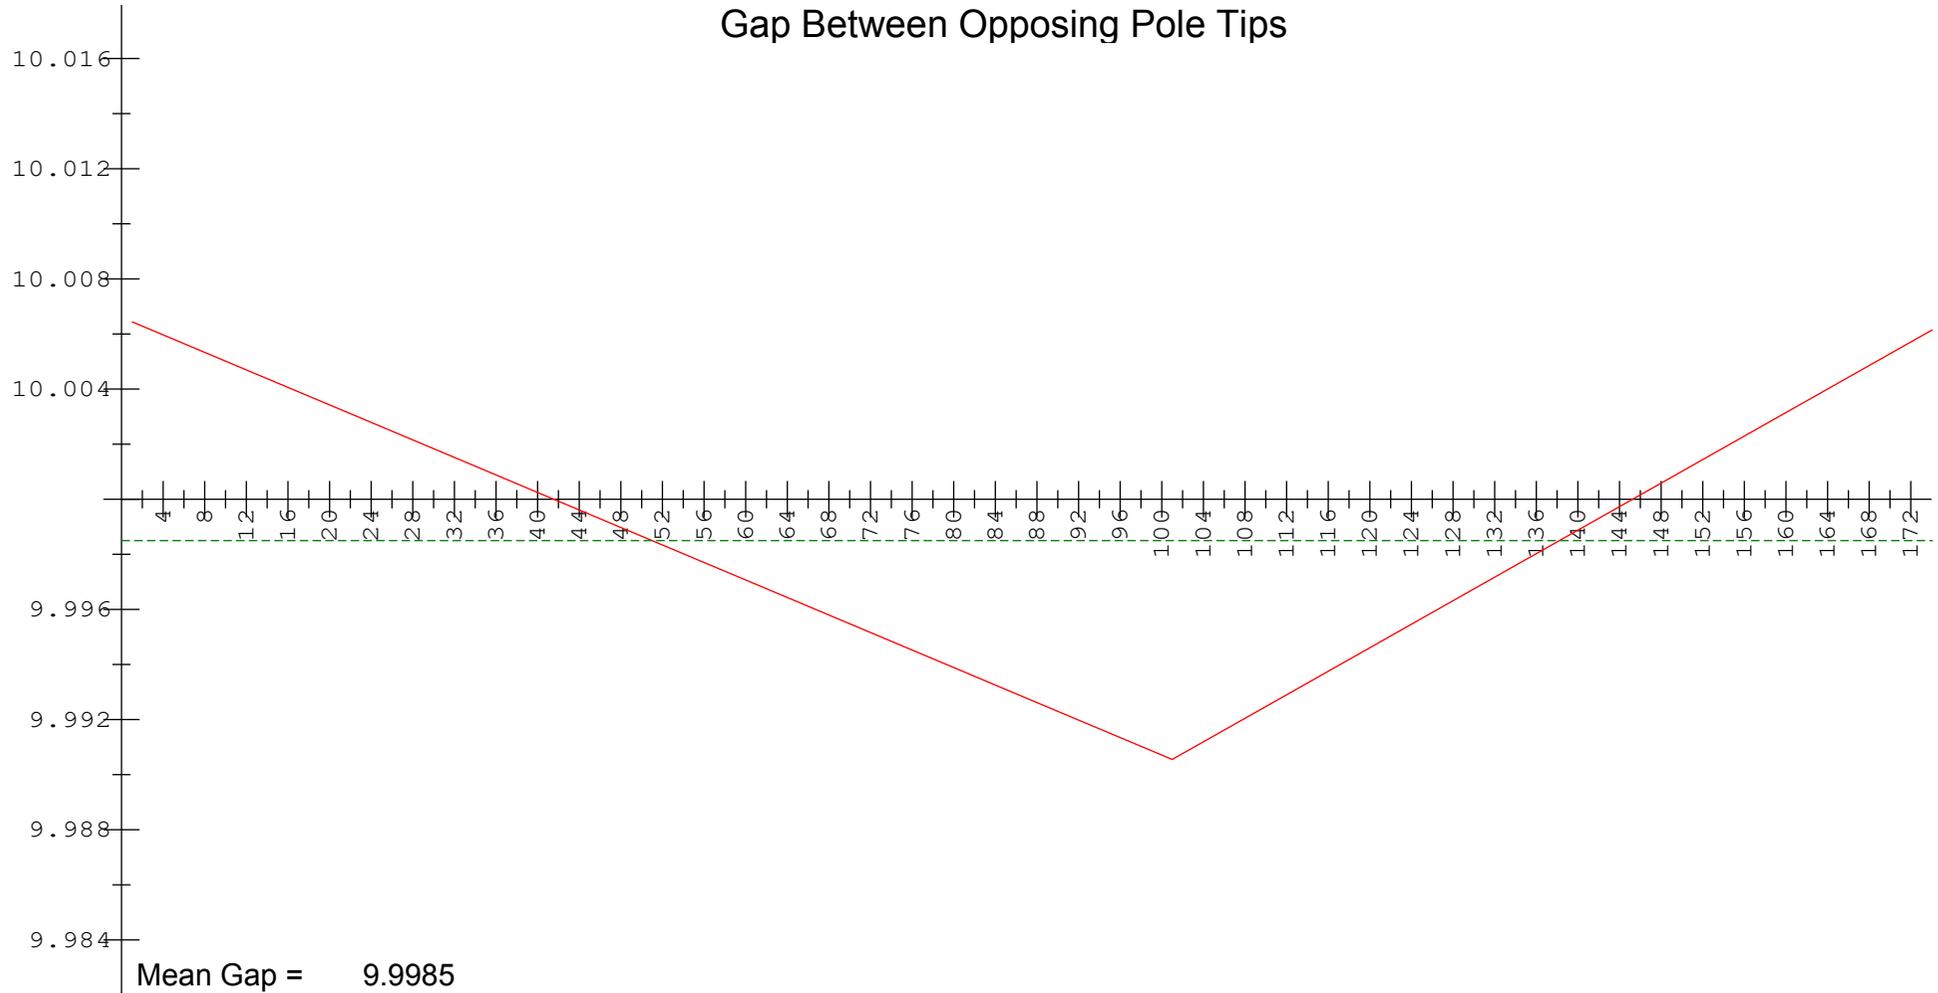

Step Between Measured Pole Tips = 100


Dimensions in mm



LCLS II - SXR Undulator

Nominal Gap = 10 Nominal Taper = 0.000
 Gap Reading = 0.0000 US Encoder = 0.0000 DS Encoder = 0.0000

30-JUL-2019
 S/N = 001
 D/S = 0007
 Run = 8

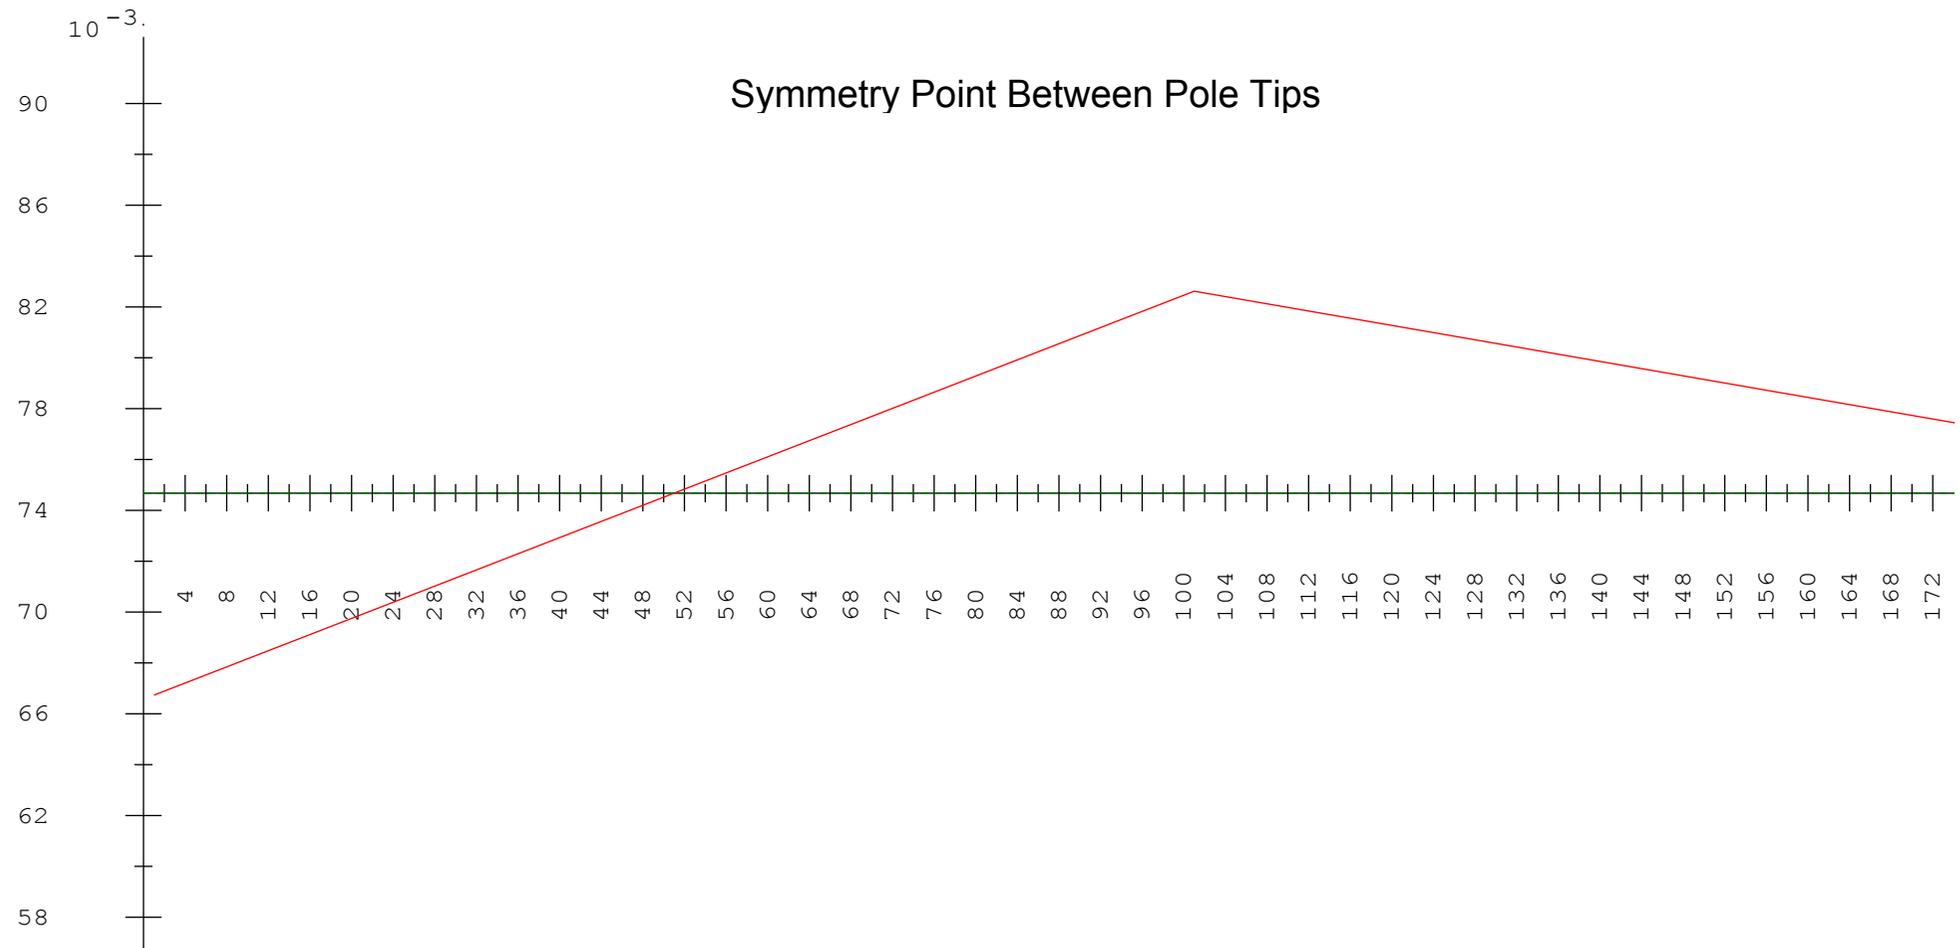

Mean Symmetry Value = 0.0747

Step Between Measured Pole Tips = 100

Dimensions in mm



LCLS II - SXR Undulator

Nominal Gap = 10 Nominal Taper = 0.000
 Gap Reading = 0.0000 US Encoder = 0.0000 DS Encoder = 0.0000

30-JUL-2019
 S/N = 001
 D/S = 0007
 Run = 8

Top and Bottom Jaw Regression Line Intersect Points

Jaw	First Pole (Pole 1)	US Actuator (Pole 39)	DS Actuator (Pole 135)	Last Pole (Pole 174)
Top	5.0705	5.0728	5.0788	5.0812
Bottom	-4.9316	-4.9288	-4.9218	-4.9189
Gap	10.0021			10.0001
Taper				-0.0019

Summary of Mean Values

Top Jaw Poles	Btm. Jaw Poles	Gap Values	Sym. Pt. Values
5.0739	-4.9246	9.9985	0.0747

Additional Calculated Values

Bottom Pole #1 Z Value	980.085
Top Jaw Pitch (mrad)	0.003
Bottom Jaw Pitch(mrad)	0.004
Minimum Effective Gap	9.983
Reference Block Gap	6.804

Dimensions in mm



LCLS II - SXR Undulator

Nominal Gap = 10 Nominal Taper = 0.000
 Gap Reading = 0.0000 US Encoder = 0.0000 DS Encoder = 0.0000

30-JUL-2019
 S/N = 001
 D/S = 0007
 Run = 8