



GLAST Repeatability Results

Laser Tracker Study in SLAC
Building 33 - Room 104


High Position Laser Tracker Repeatability Study Observing Target "Stand" Horizontal Angle Readings

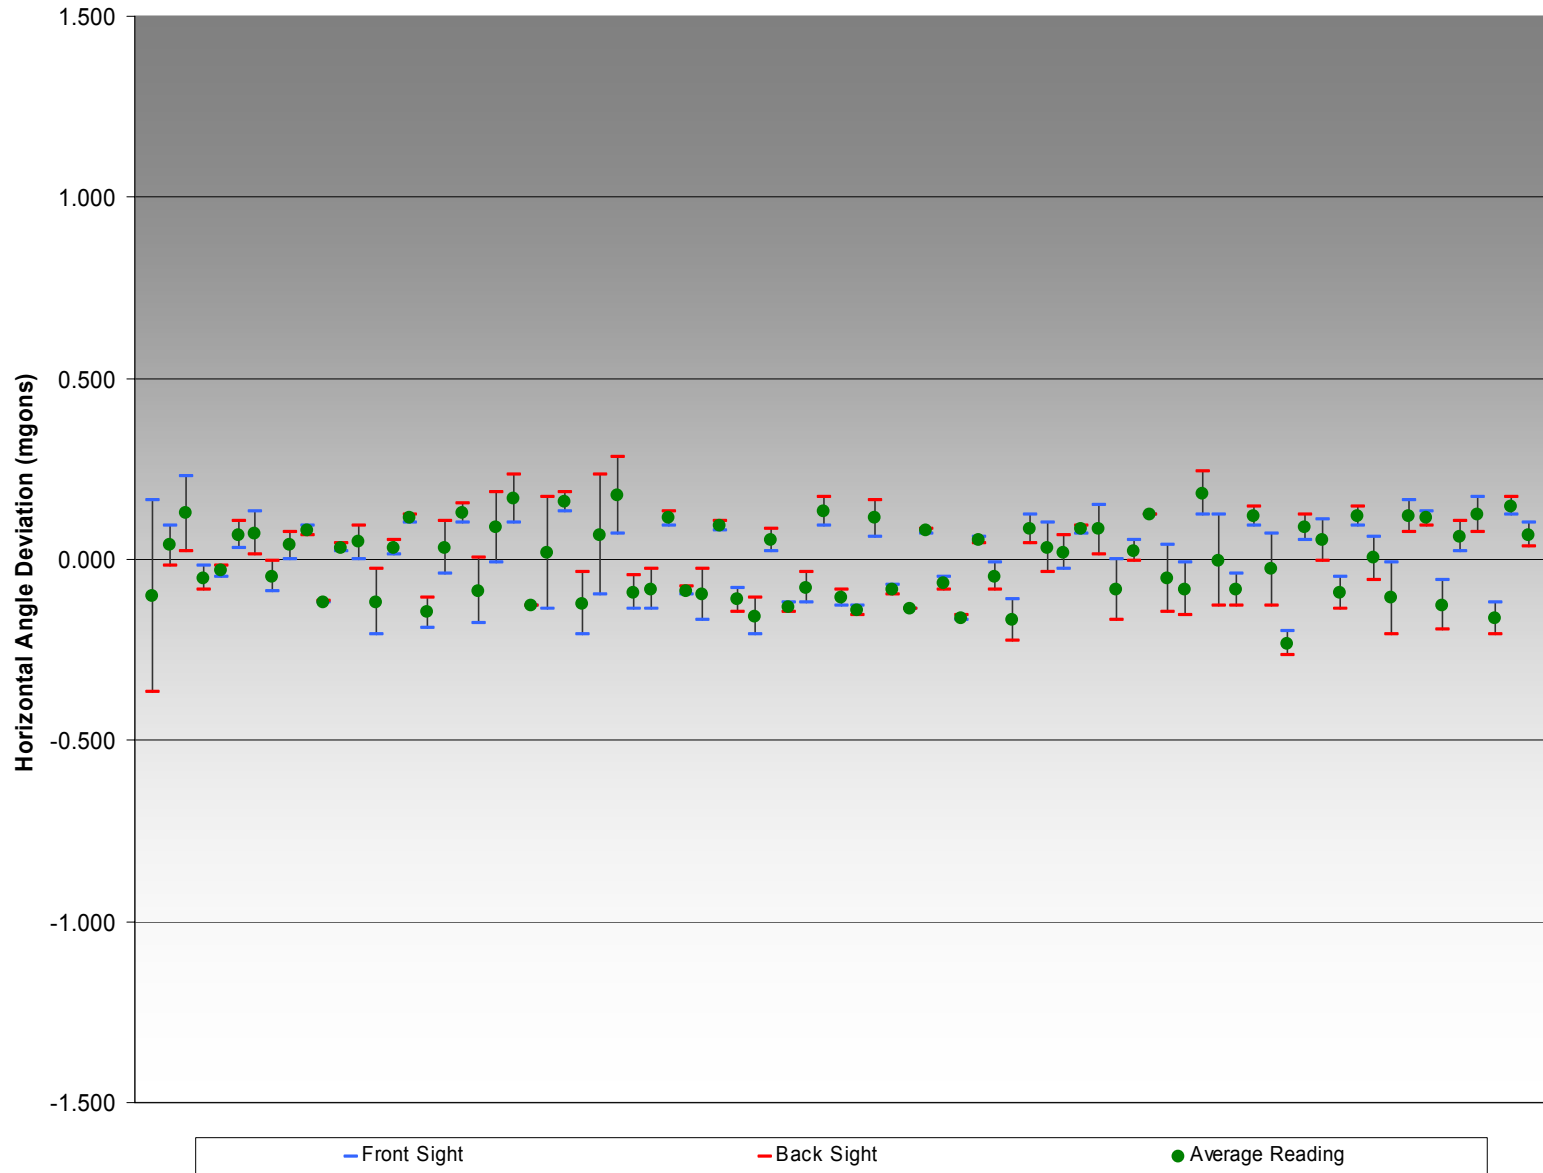


High Position Laser Tracker Repeatability Study Observing Target "Stand" Slope Distance Readings

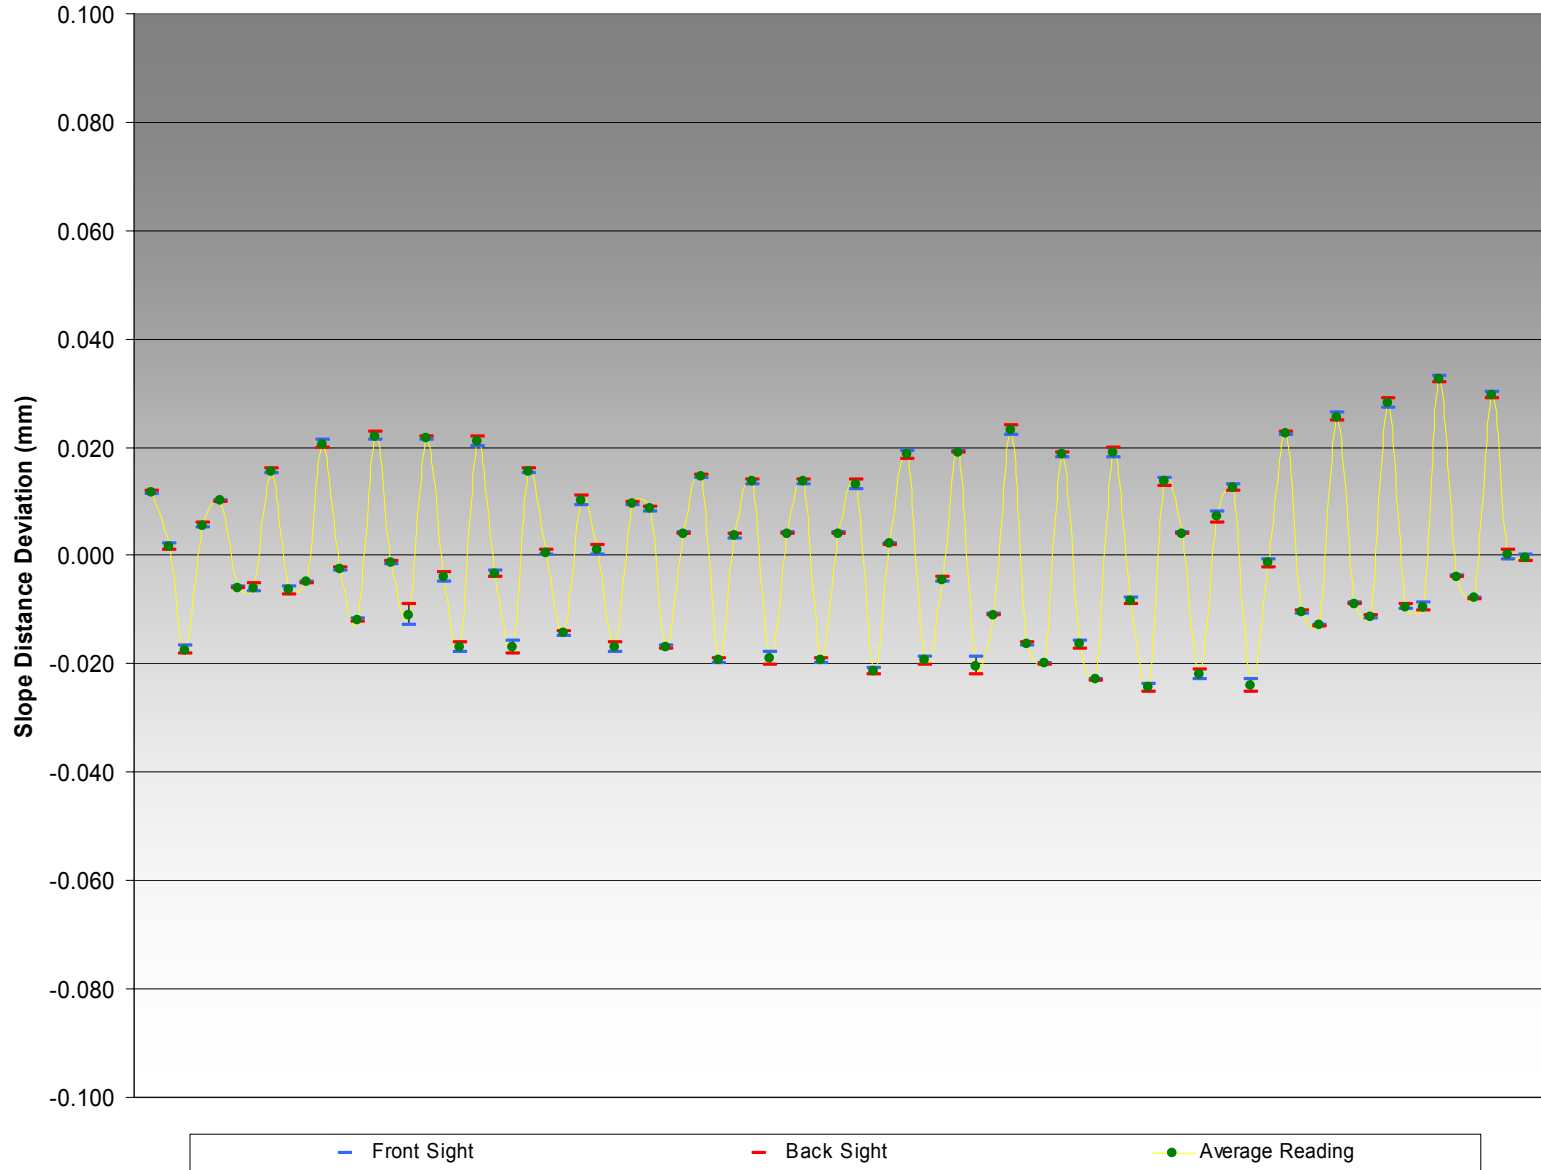


High Position Laser Tracker Repeatability Study Horizontal Angle Readings

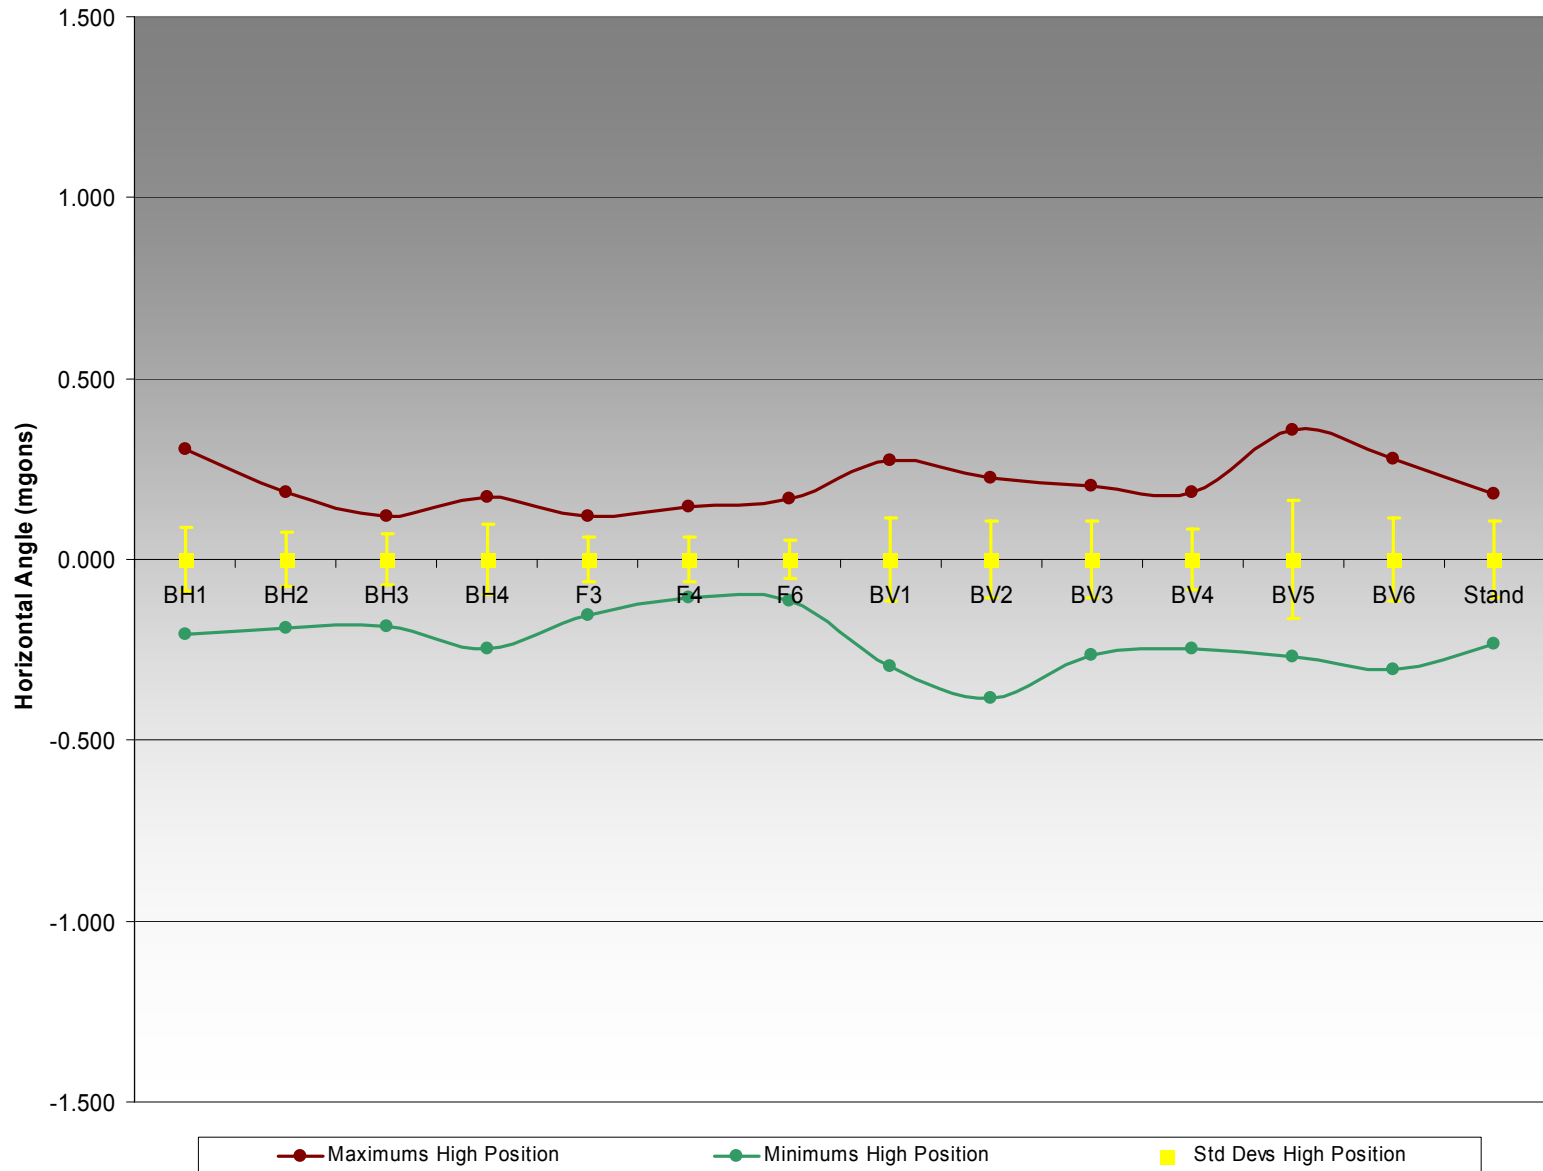


High Position Laser Tracker Repeatability Study Zenith Angle Readings

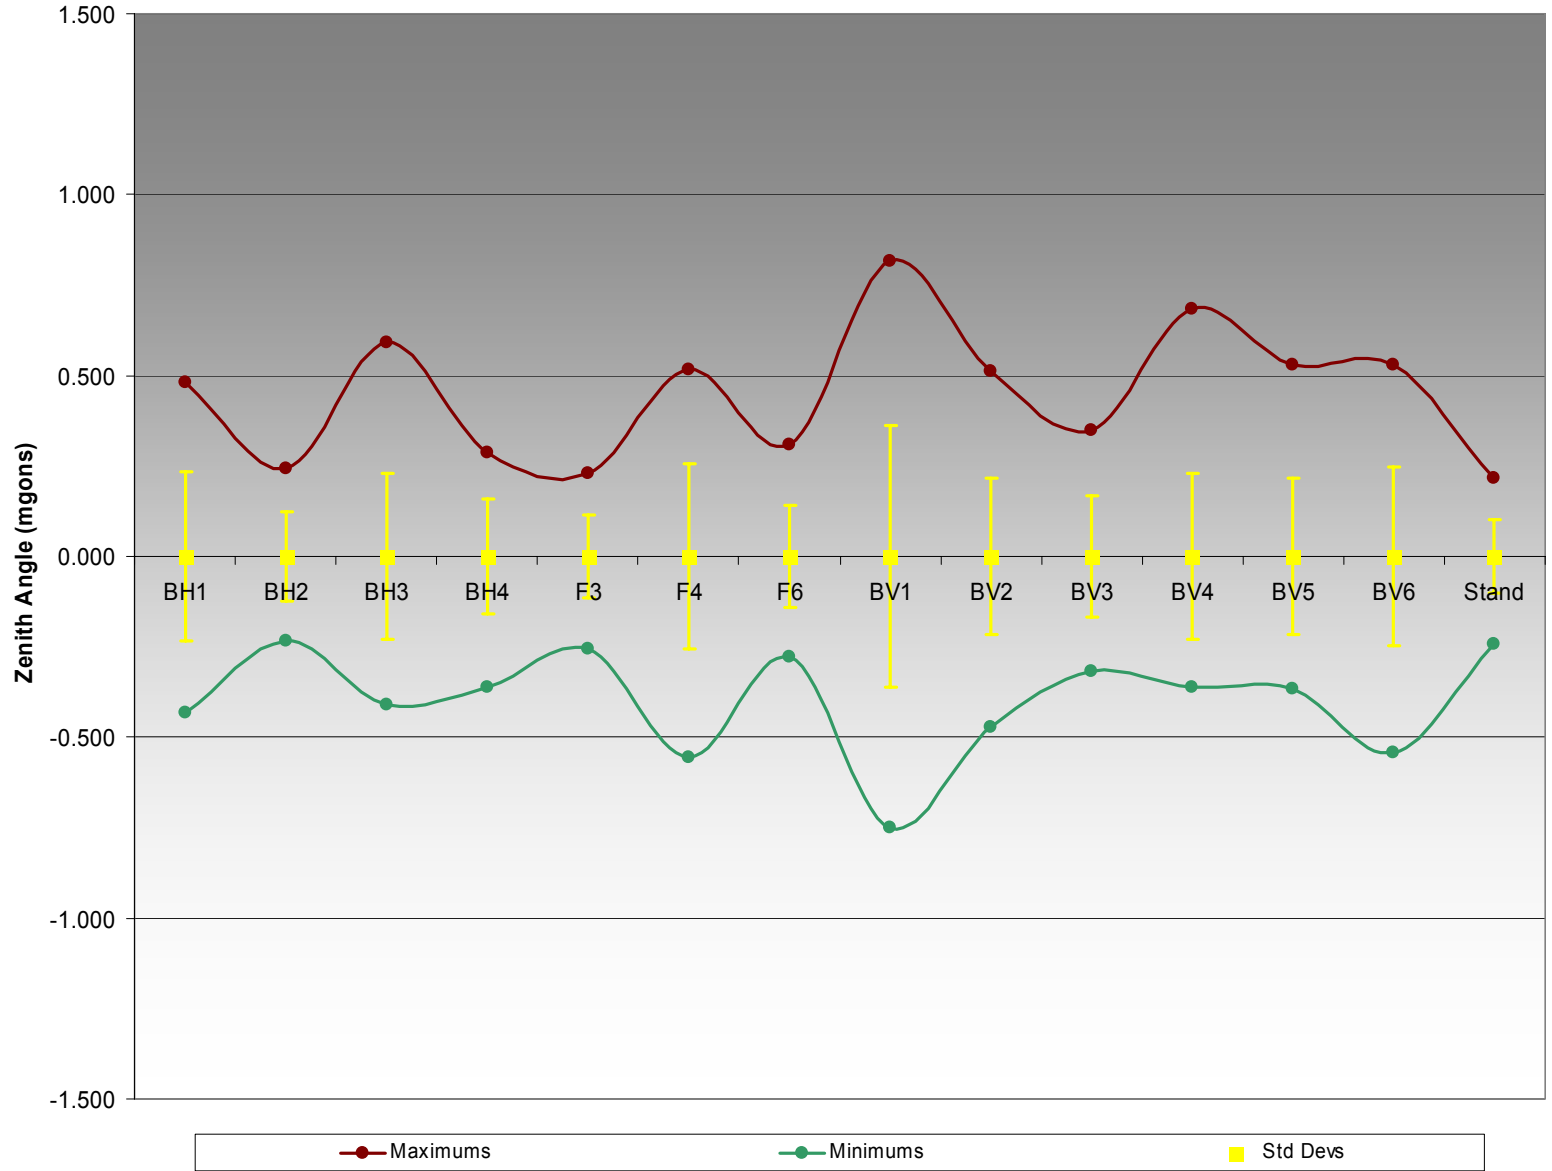


High Position Laser Tracker Repeatability Study Slope Distance Readings

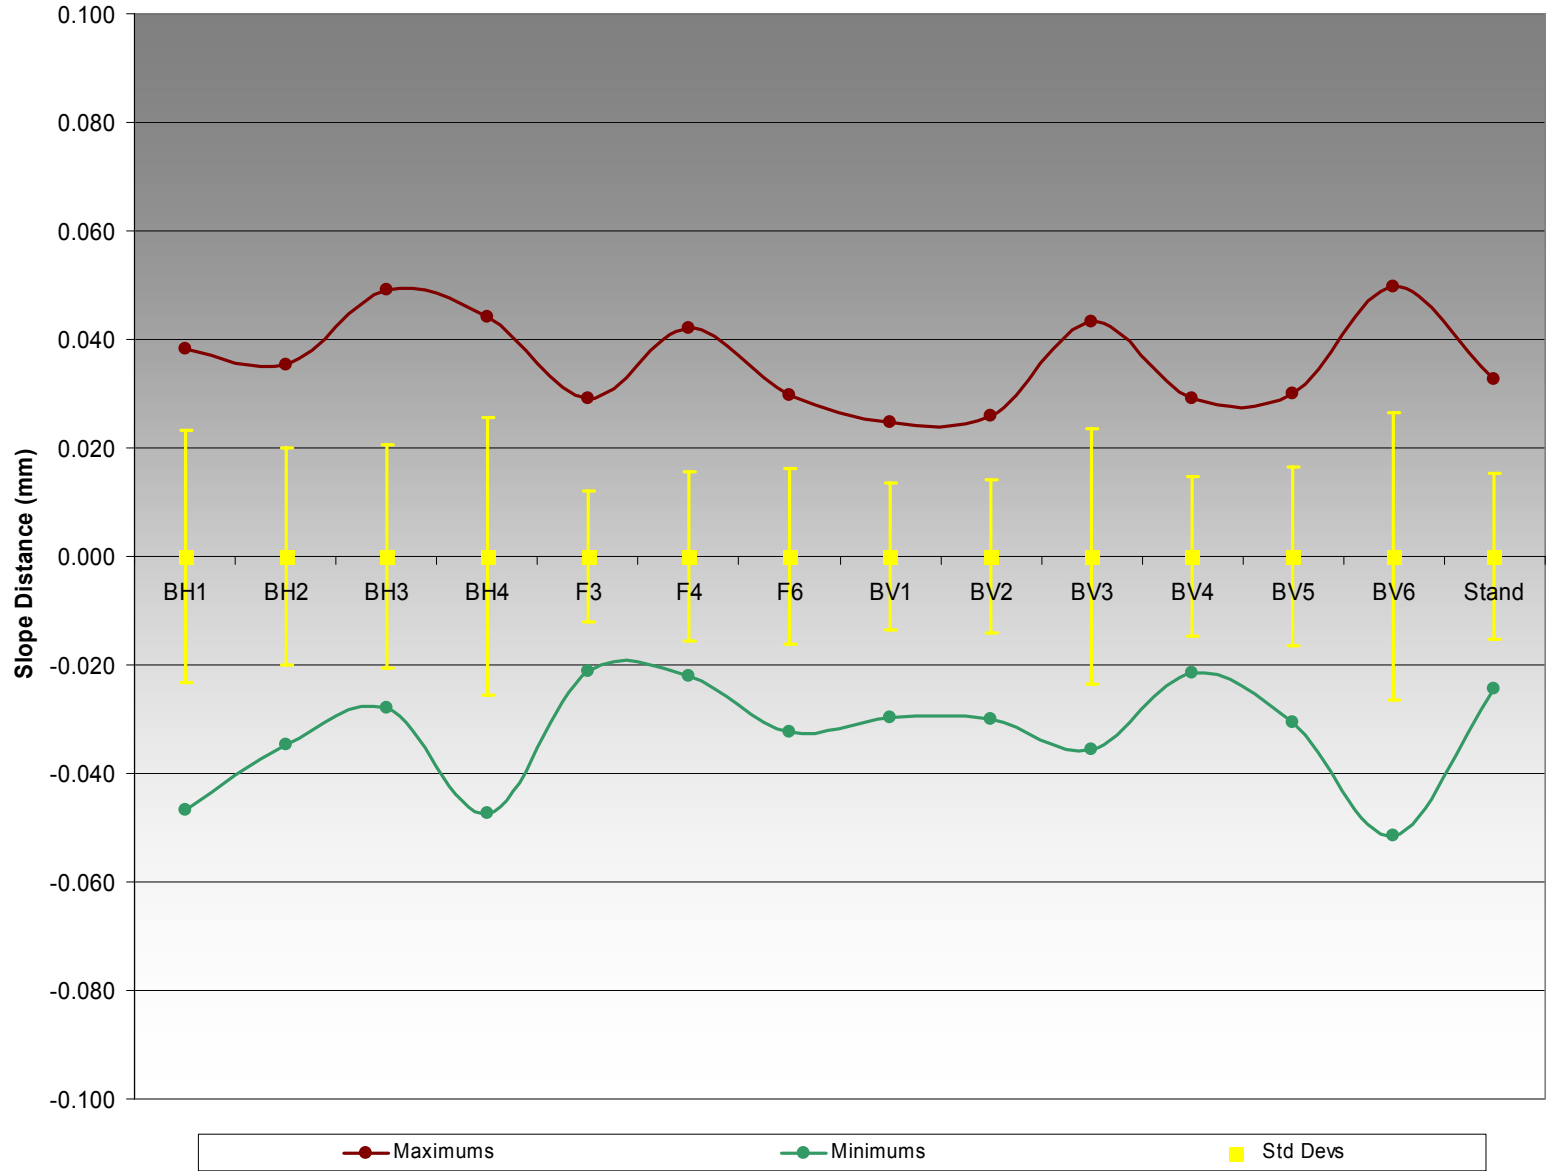


Low Position Laser Tracker Repeatability Study Observing Target "Stand" Horizontal Angle Readings

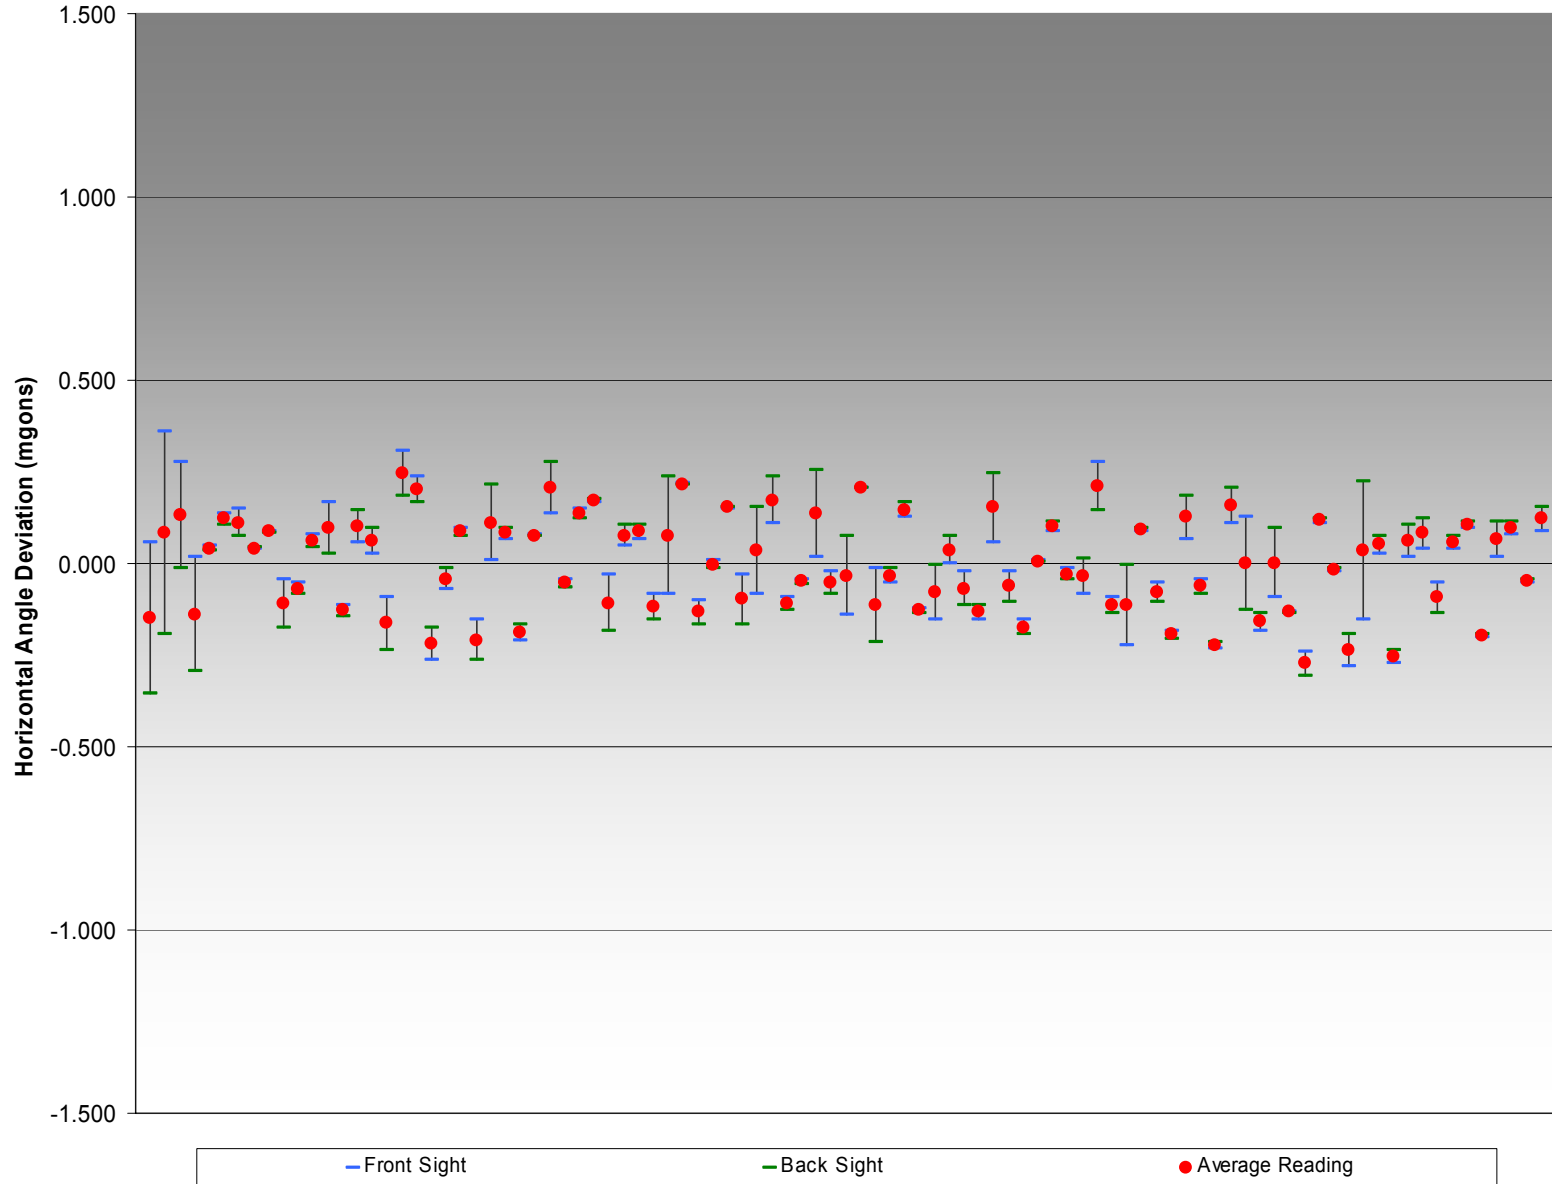


Low Position Laser Tracker Repeatability Study Observing Target "Stand" Zenith Angle Readings

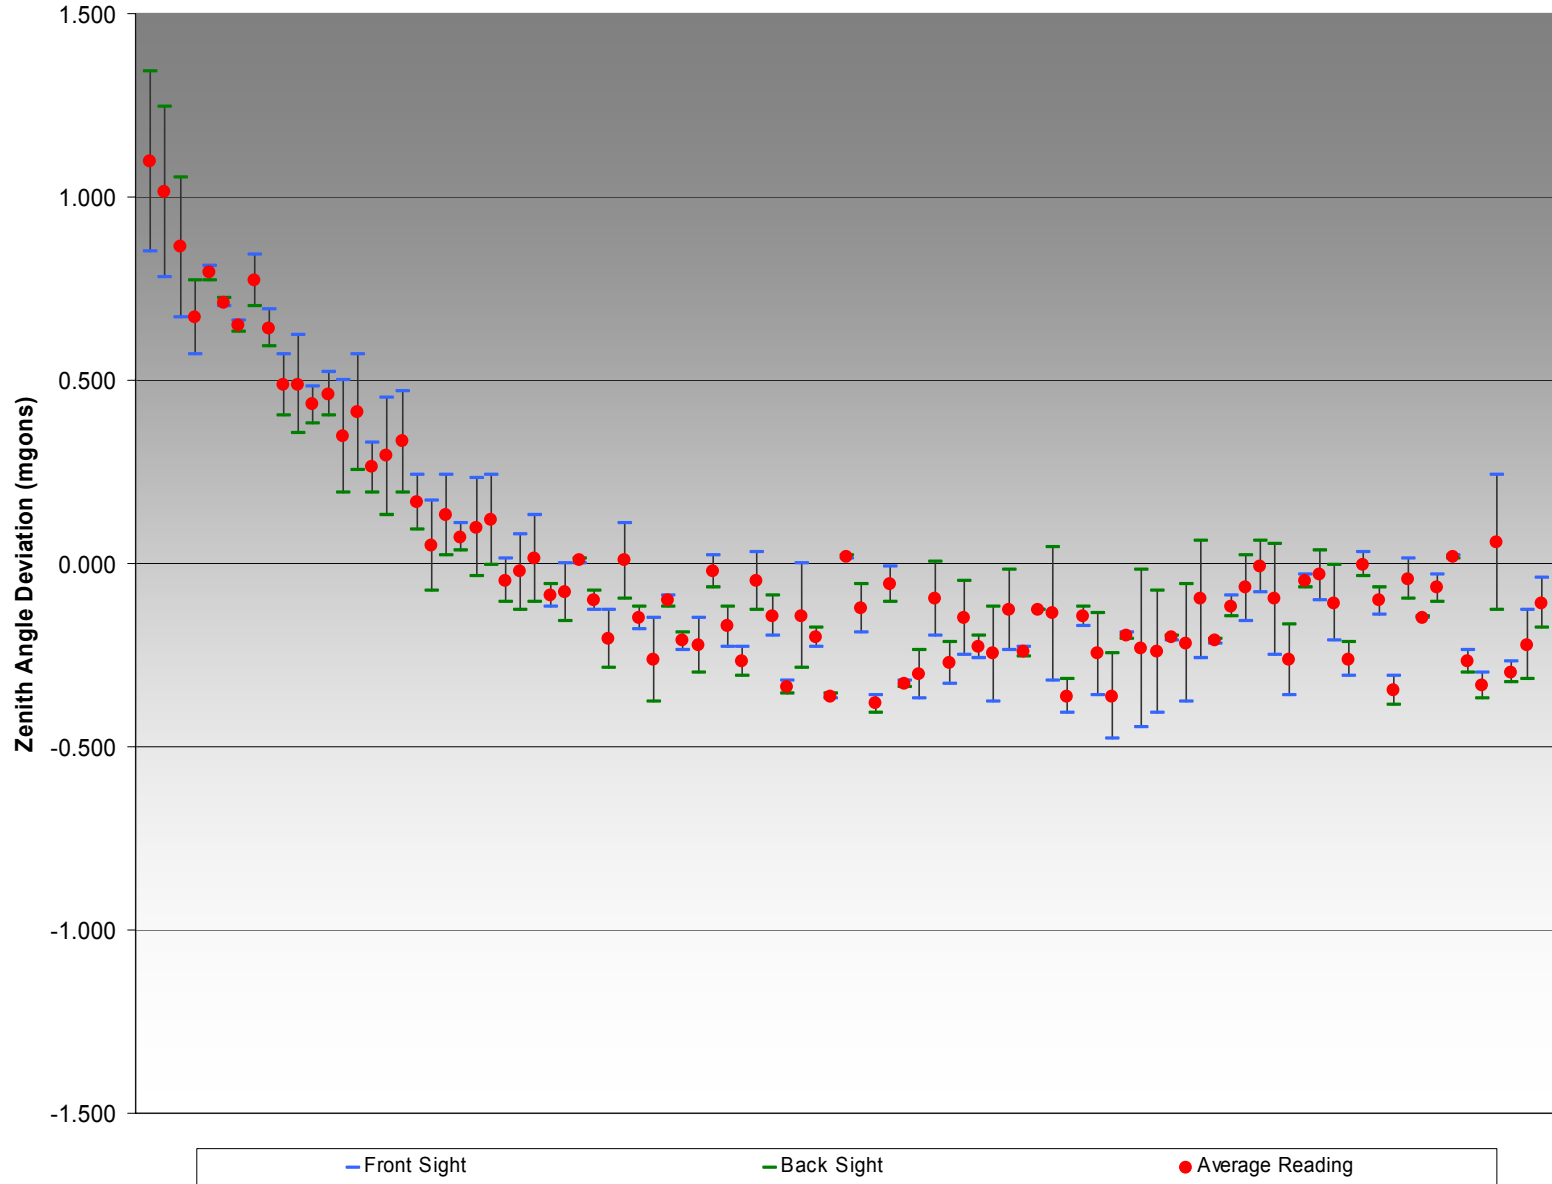


Low Position Laser Tracker Repeatability Study Observing Target "Stand" Slope Distance Readings

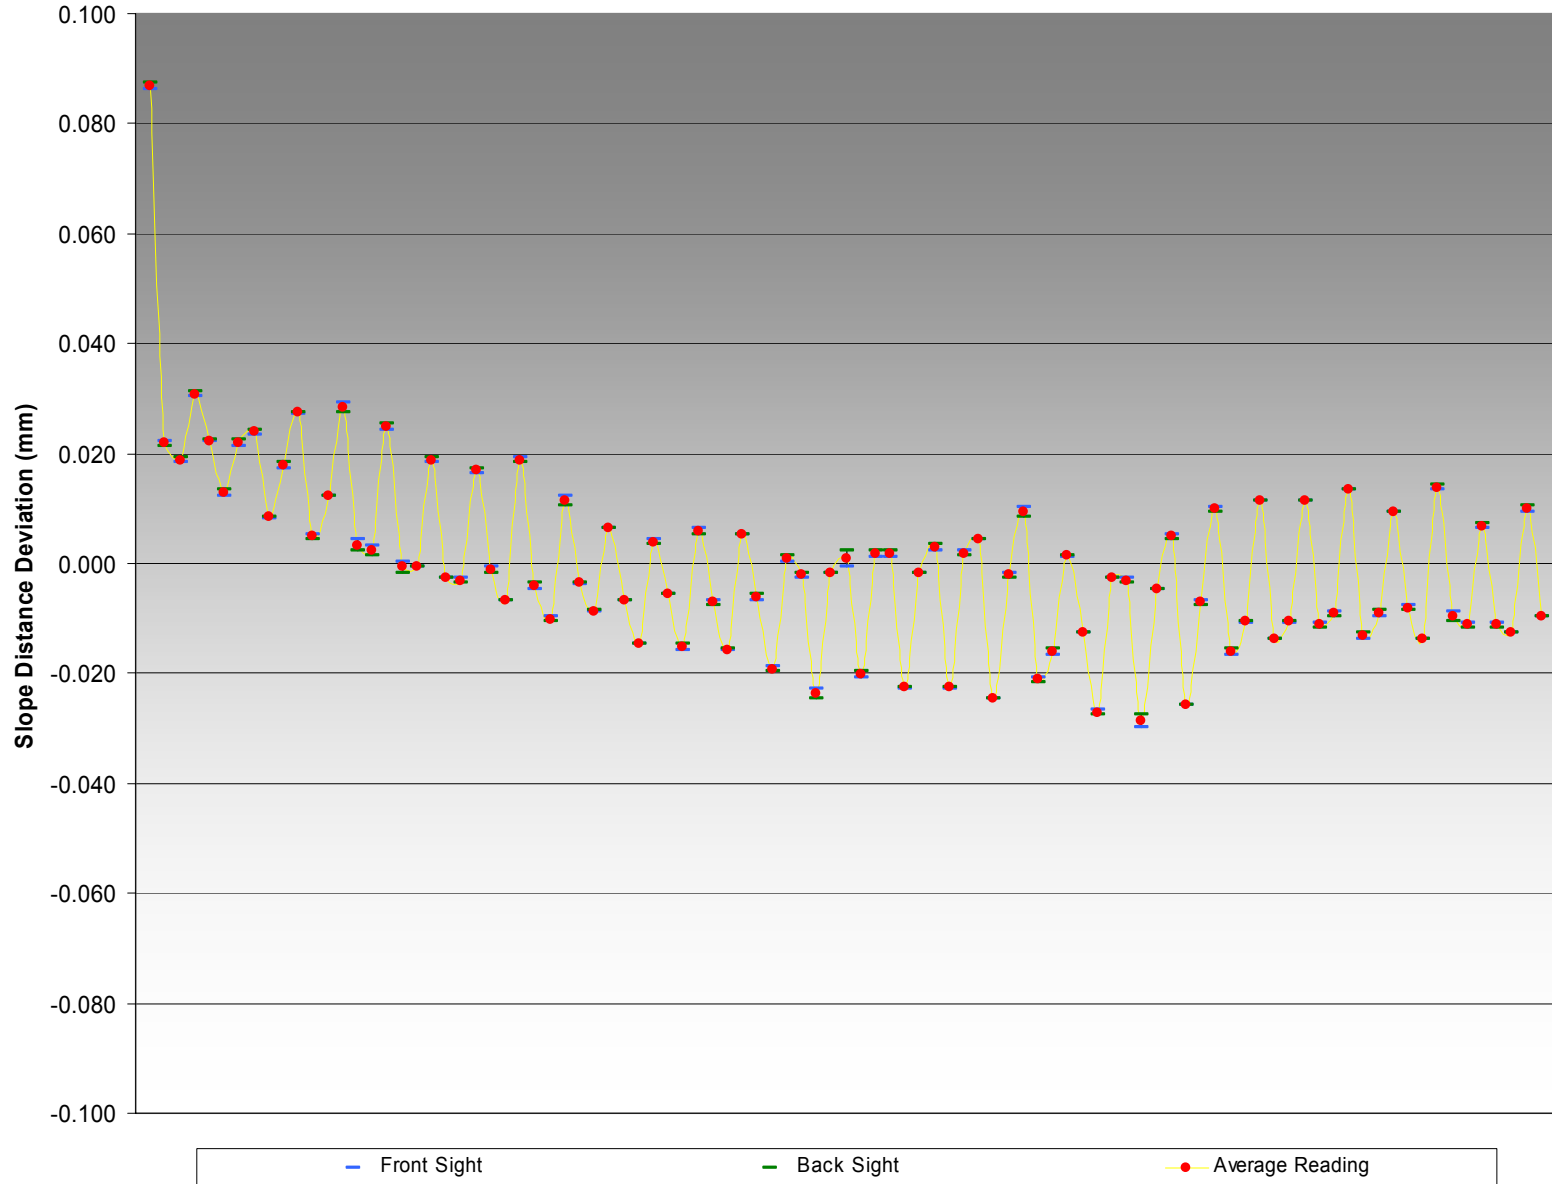


Low Position Laser Tracker Repeatability Study Horizontal Angle Readings

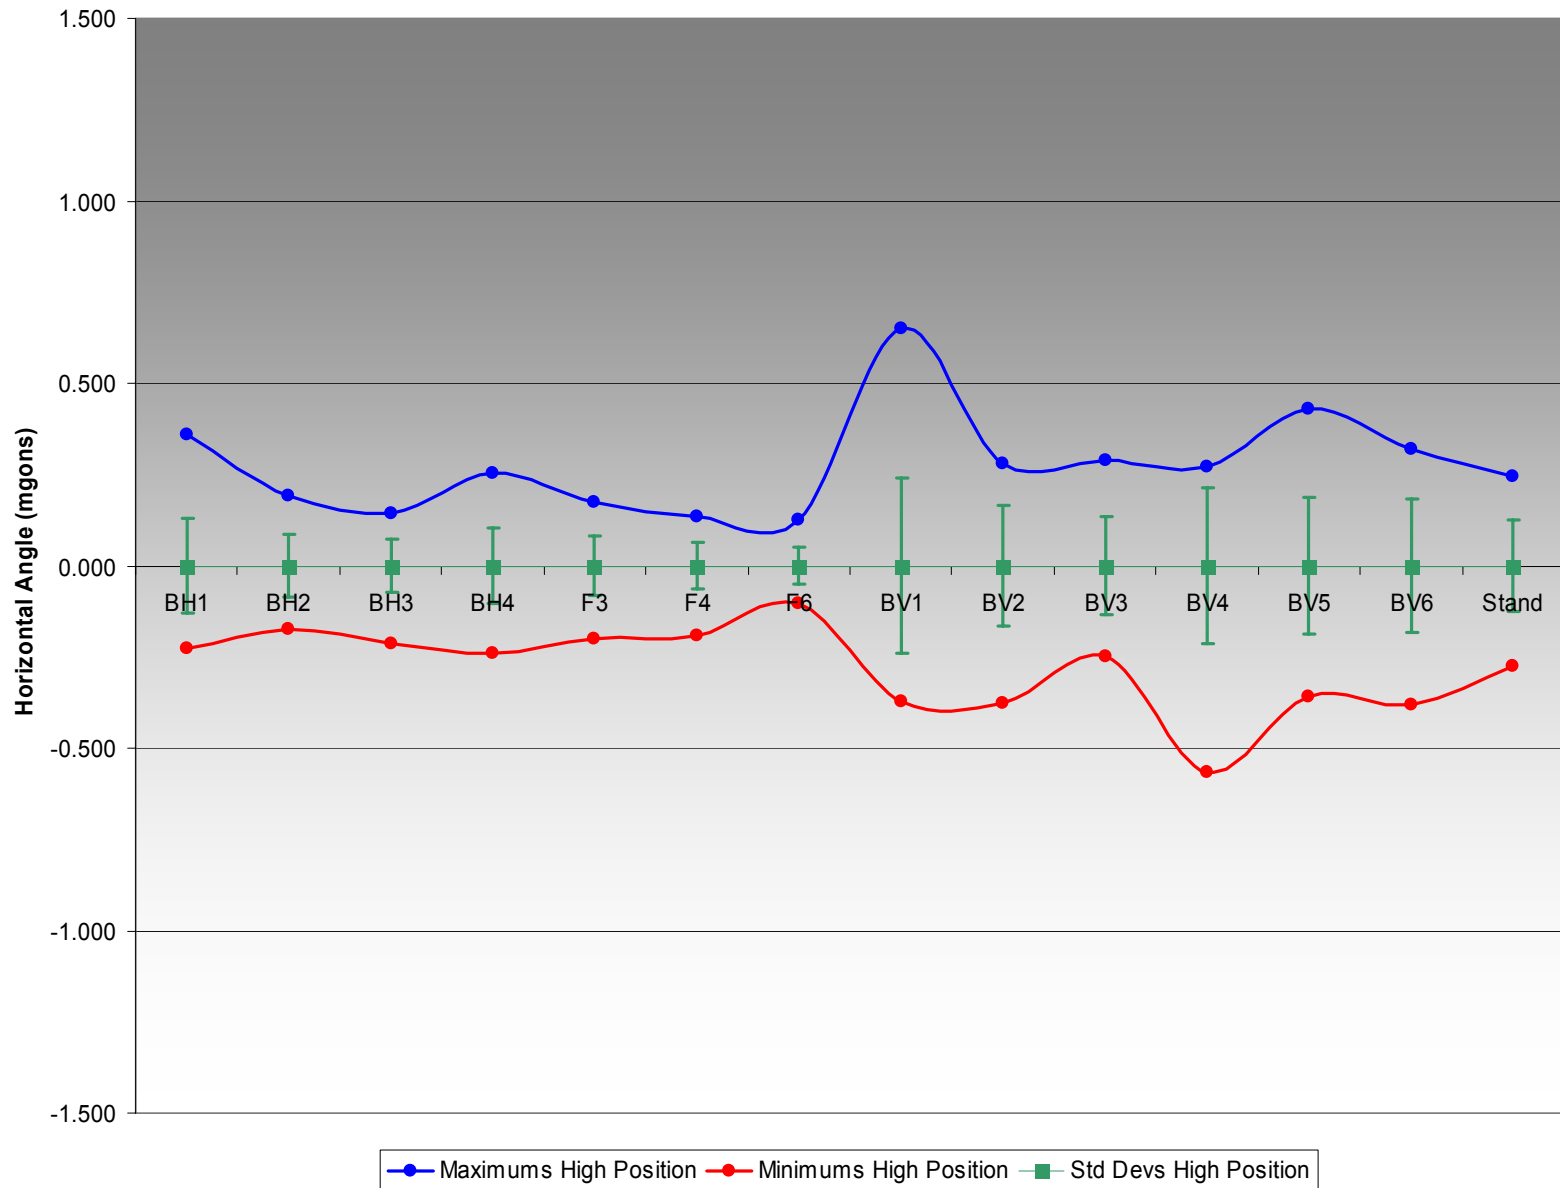


Low Position Laser Tracker Repeatability Study Zenith Angle Readings

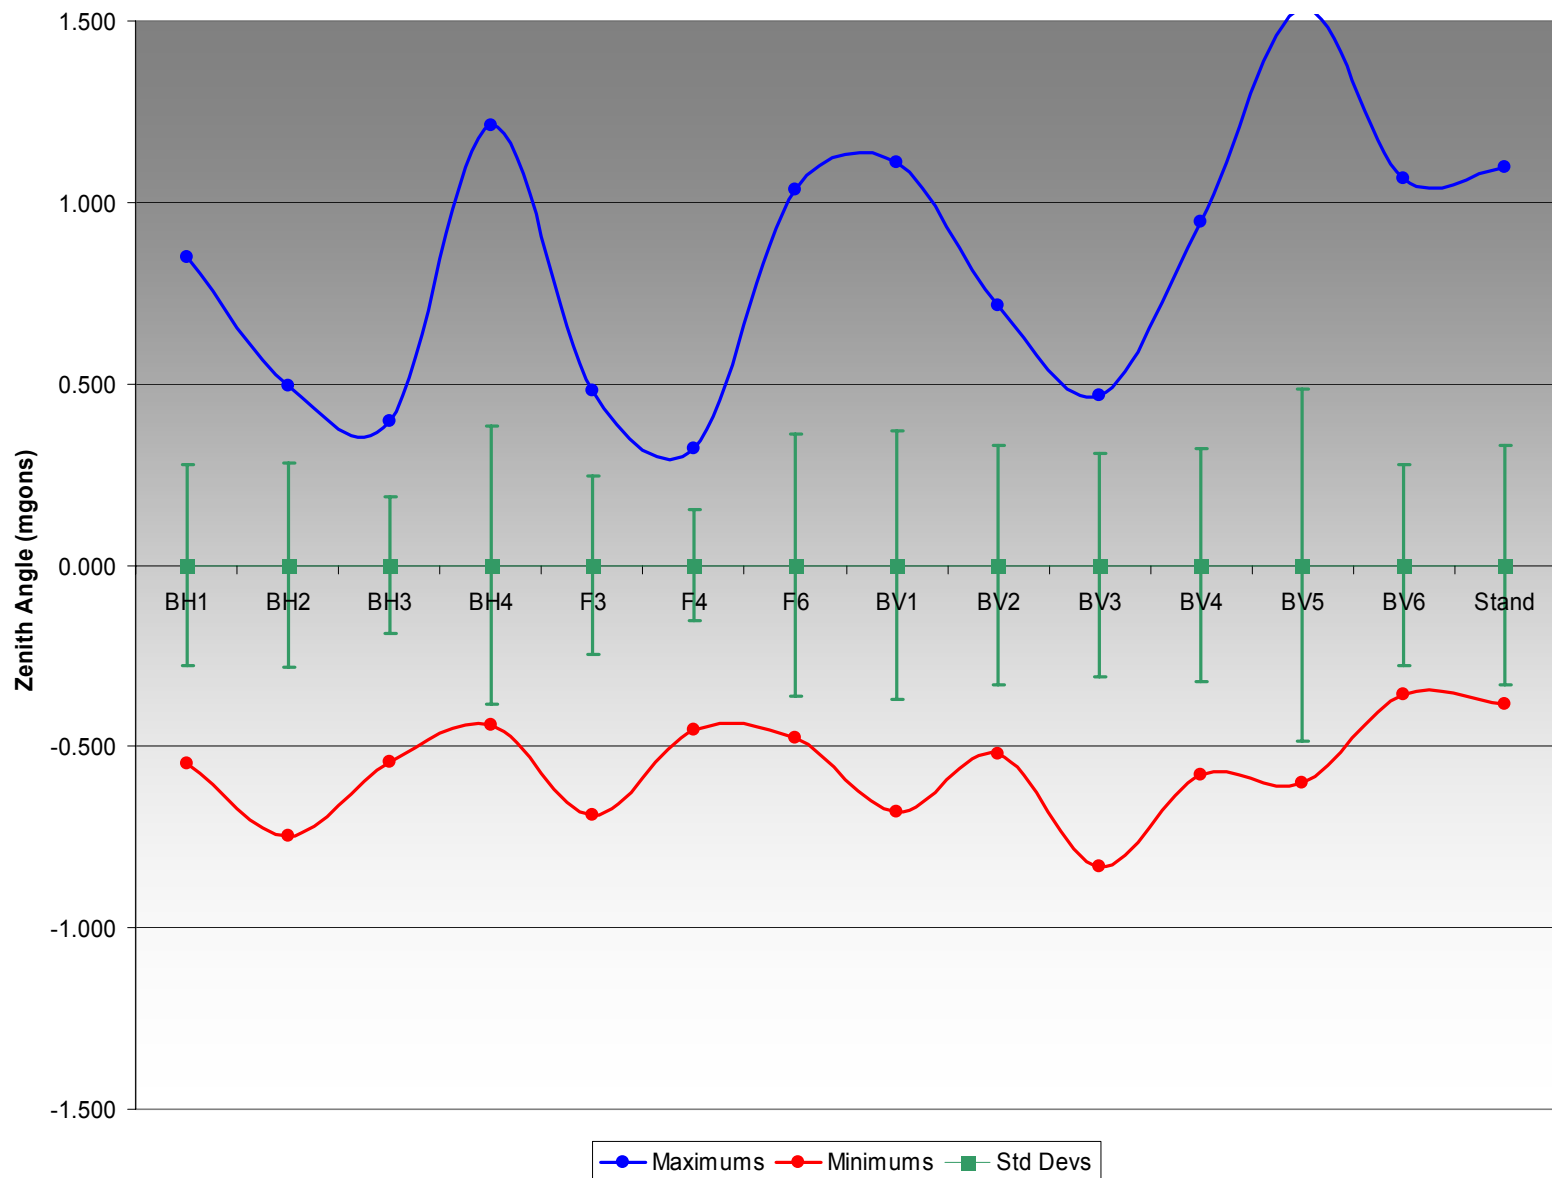

Low Position Laser Tracker Repeatability Study Slope Distance Readings

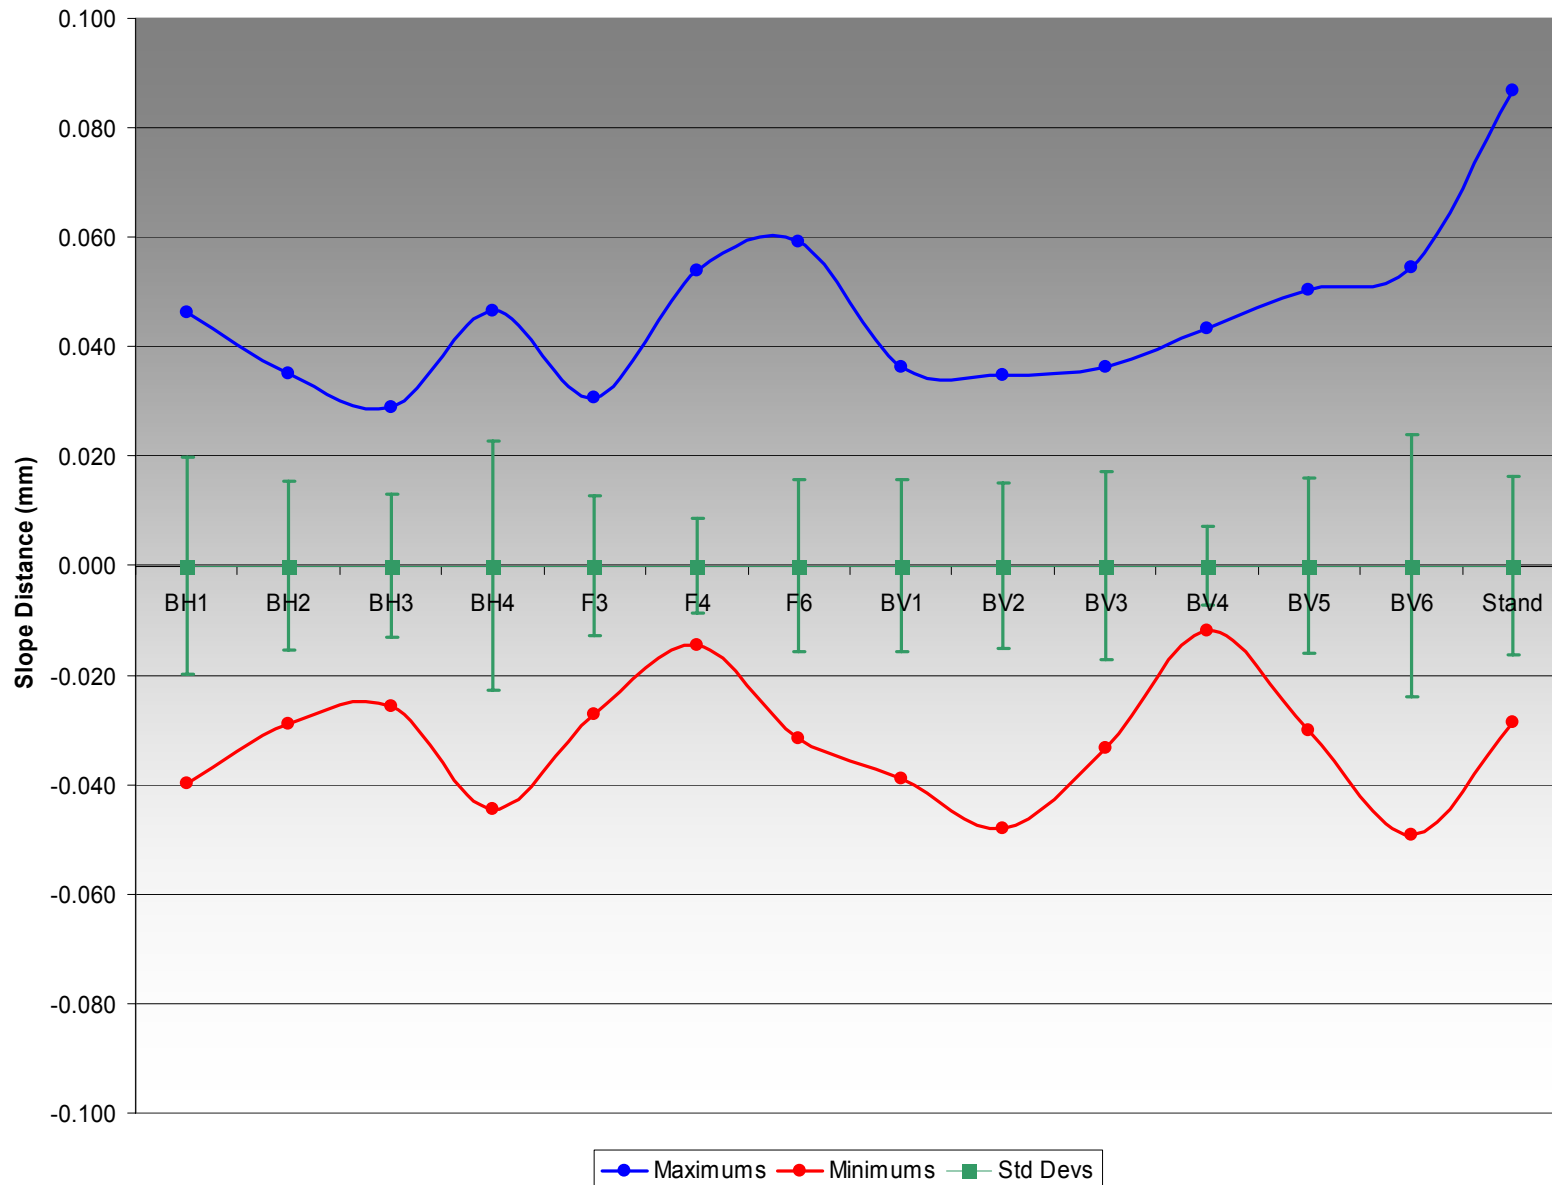


Bld 33 Cleanroom Temperature (1-week)

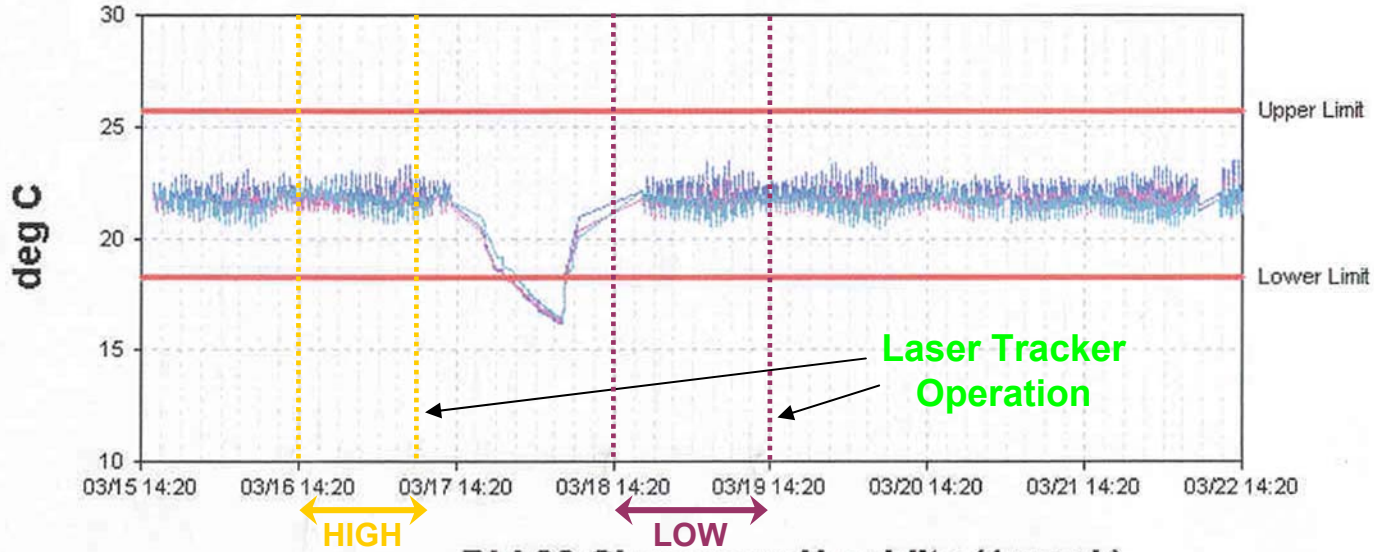

Top Plots

- TEMP-01
- TEMP-02
- TEMP-05

Bld 33 Cleanroom Humidity (1-week)

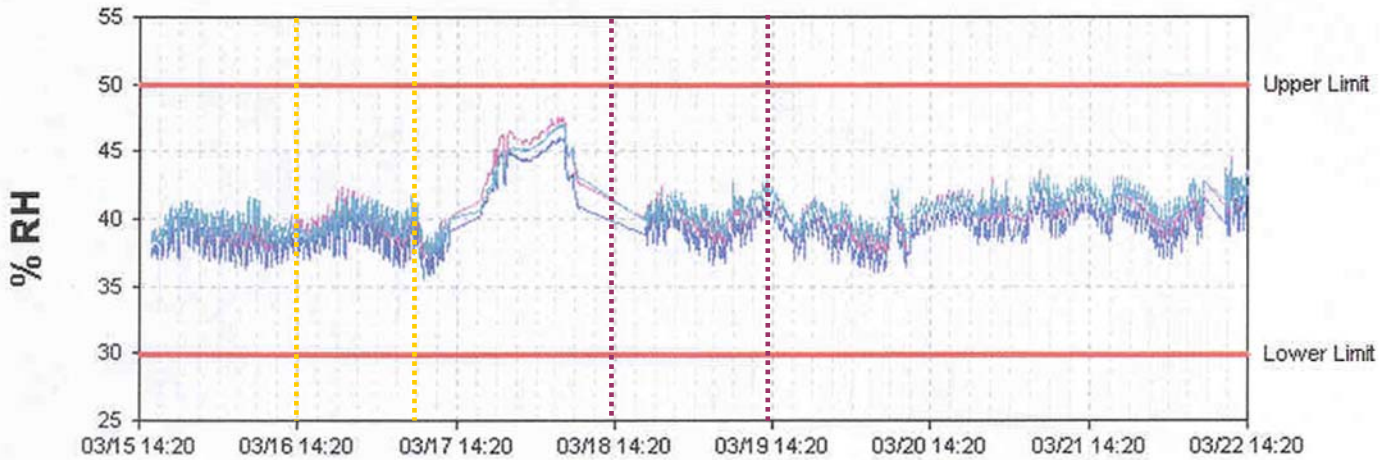

Bottom Plots

- HUM-01
- HUM-02
- HUM-05

Time: 03/15/04 14:20:55 to 03/22/04 14:20:55, Duration: 7 days + 00:00:00