SLAC Magnetic Measurements
Hall Probe Calibration

Header:
SLAC Magnetic Measurements
Date: 09-17-2018
Time: 08:28:53

Project: LCLS-II
Device Type: Hall probe
Data Type: Y
Serial Number: SENTRON-463
Run Number: 7
Measurement Type: HPCS
Operator: YL
Comment: PC71024; +6.00006, -6.00006, +1.00002

Current(A) T(C) Case T-V Est. Field(T) Voltage Voltage-T-Corr Field

Parameters:
INPUT-FILE-DIR =t:\magdata\LCLS-II\Hall probe\SENTRON-463\HPCS-007\
INPUT-FILE-NAME =hpcs-dat.001
POLY-FIT-ORDER =11
NUM-SIG-OUTLIER =2
NOM-CALIB-CONST =0.2
MAX-B-NMR-FIT =1.61

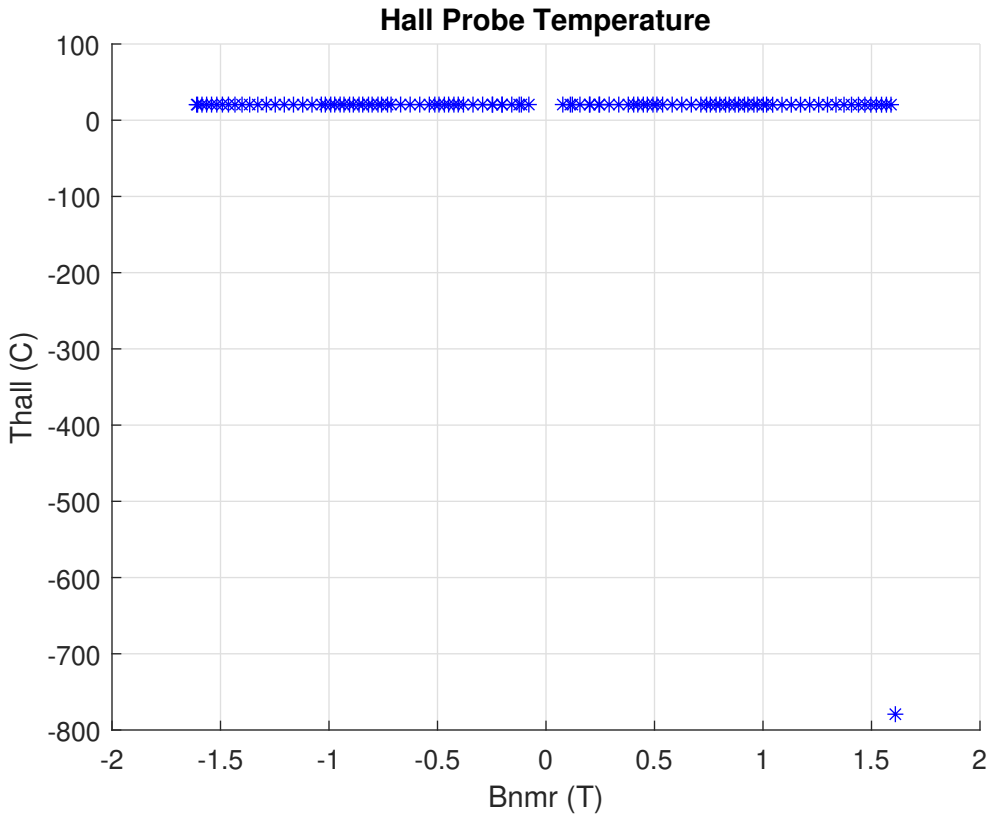
Hall Probe Temperature
100
0
-100
-200
-300
-400
-500
-600
-700
-800
Thall (C)
-2
-1.5
-1
-0.5
0
0.5
1
1.5
2
Bnmr (T)

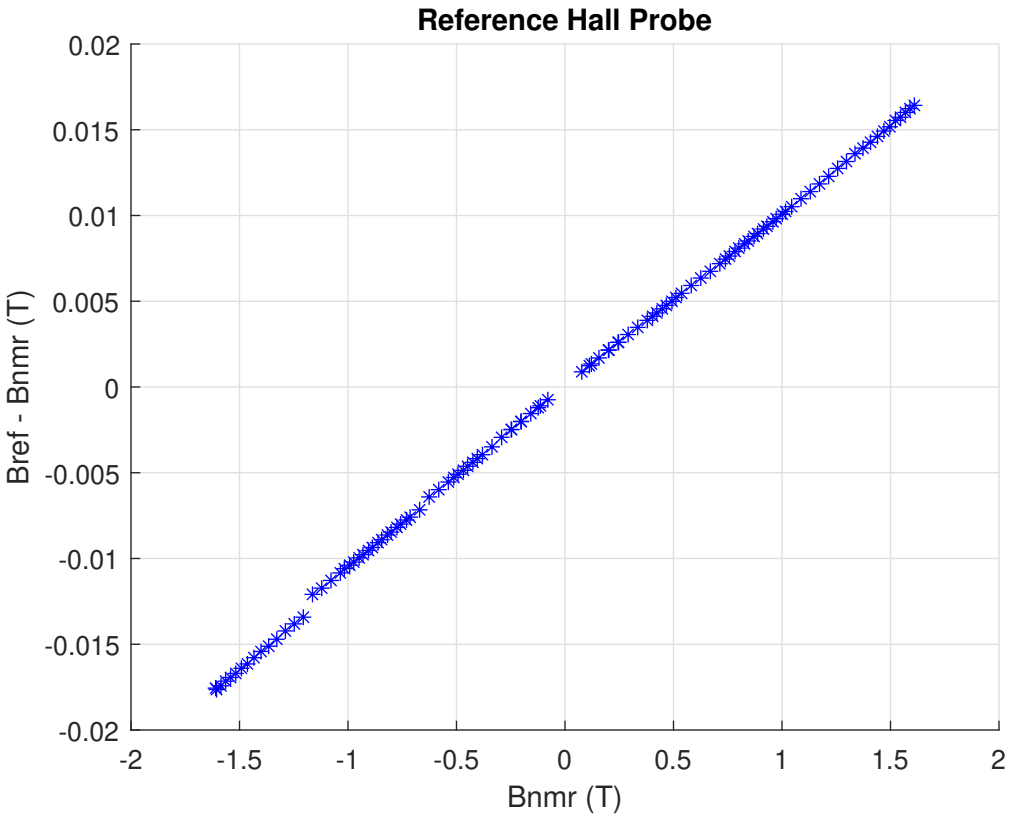
Reference Hall Probe
Bref - Bnmr (T)
Bnmr (T)
0.02
0.015
0.01
0.005
0
-0.005
-0.01
-0.015
-0.02
-2
-1.5
-1
-0.5
0
0.5
1
1.5
2

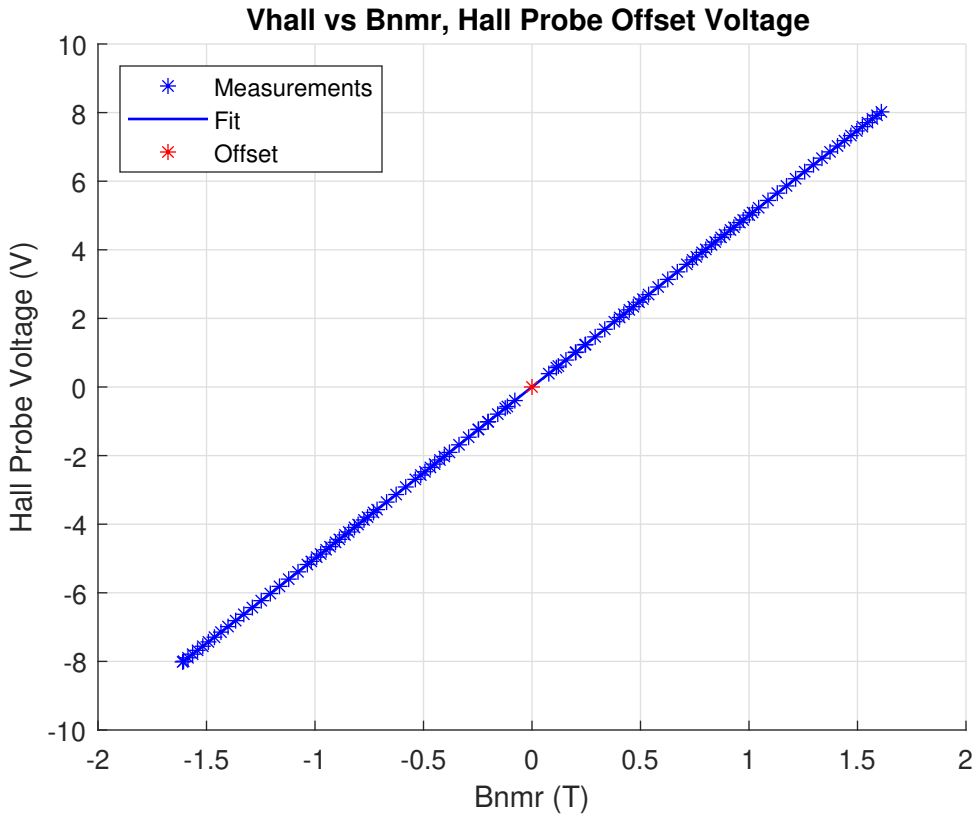
Vhall vs Bnmr, Hall Probe Offset Voltage
Measurements
Fit
Offset
Hall Probe Voltage (V)
Bnmr (T)
10
8
6
4
2
0
-2
-4
-6
-8
-10
-2
-1.5
-1
-0.5
0
0.5
1
1.5
2

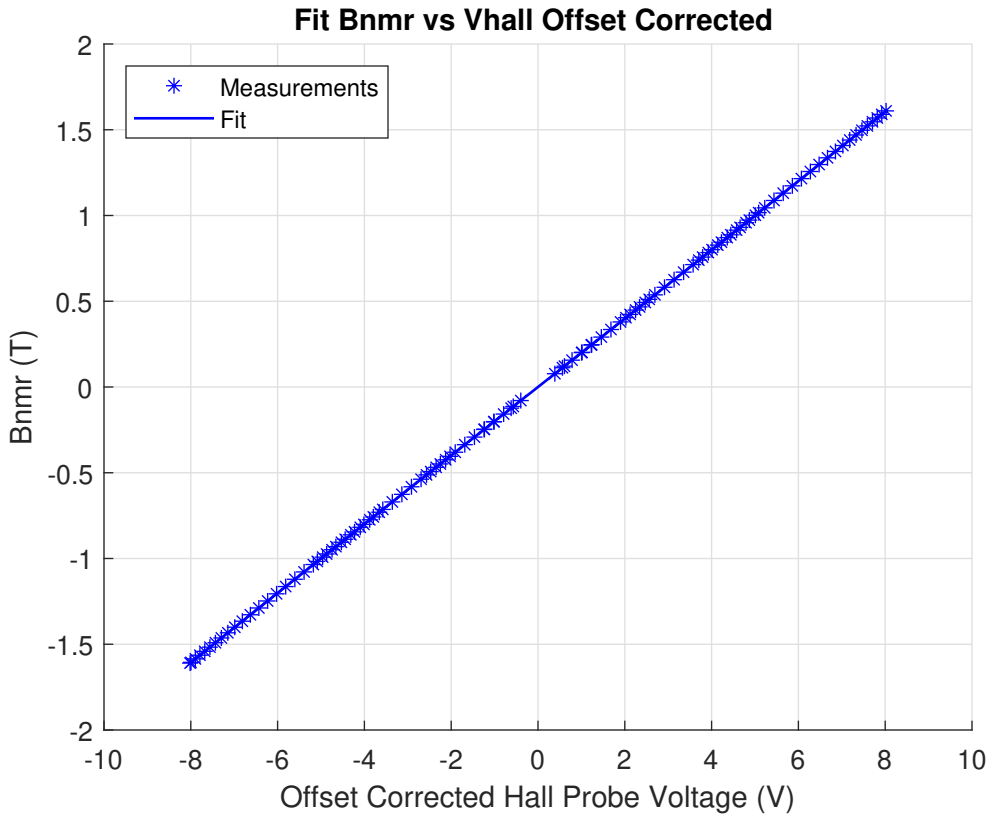
Fit Bnmr vs Vhall Offset Corrected
Measurements
Fit
Bnmr (T)
Offset Corrected Hall Probe Voltage (V)
2
1.5
1
0.5
0
-0.5
-1
-1.5
-2
-10
-8
-6
-4
-2
0
2
4
6
8
10

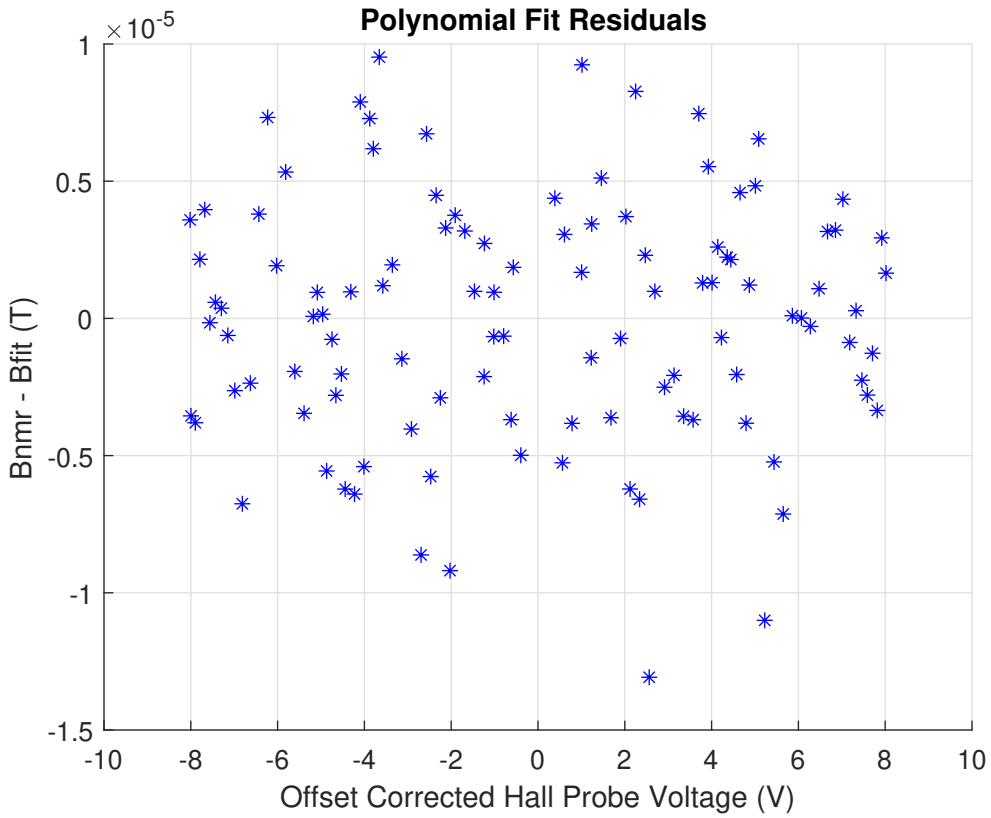
Polynomial Fit Residuals
×10^-5
1
0.5
0
-0.5
-1
-1.5
Bnmr - Bfit (T)
-10
-8
-6
-4
-2
0
2
4
6
8
10
Offset Corrected Hall Probe Voltage (V)

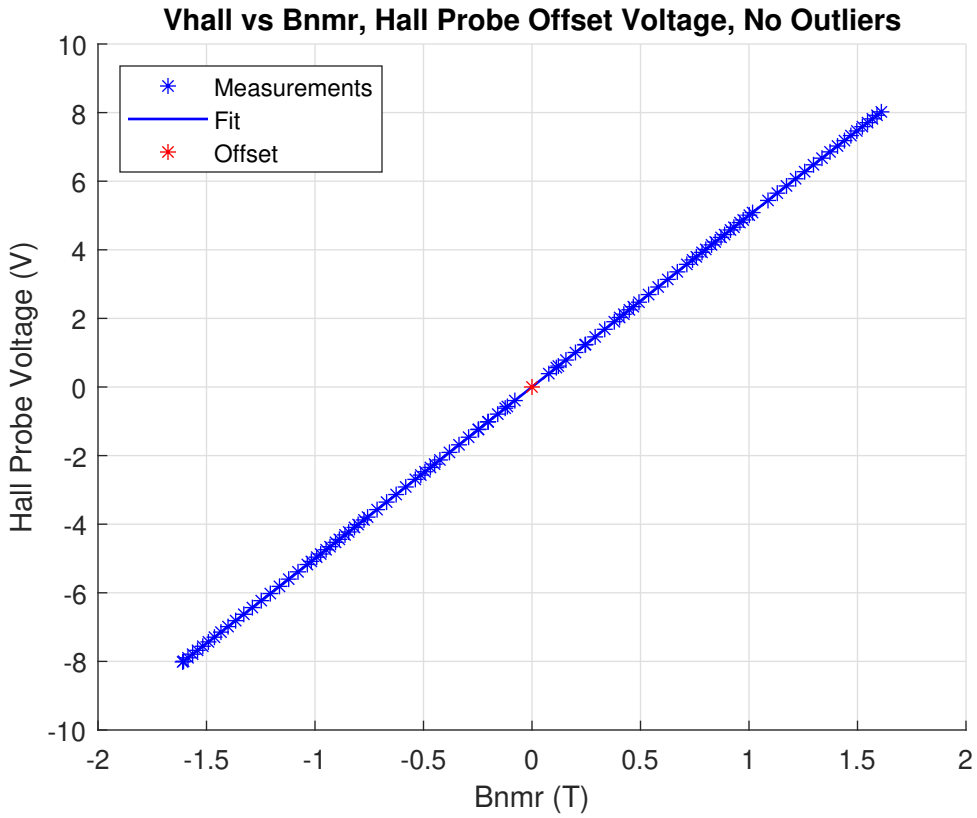
Vhall vs Bnmr, Hall Probe Offset Voltage, No Outliers
Measurements
Fit
Offset
Hall Probe Voltage (V)
Bnmr (T)
10
8
6
4
2
0
-2
-4
-6
-8
-10
-2
-1.5
-1
-0.5
0
0.5
1
1.5
2

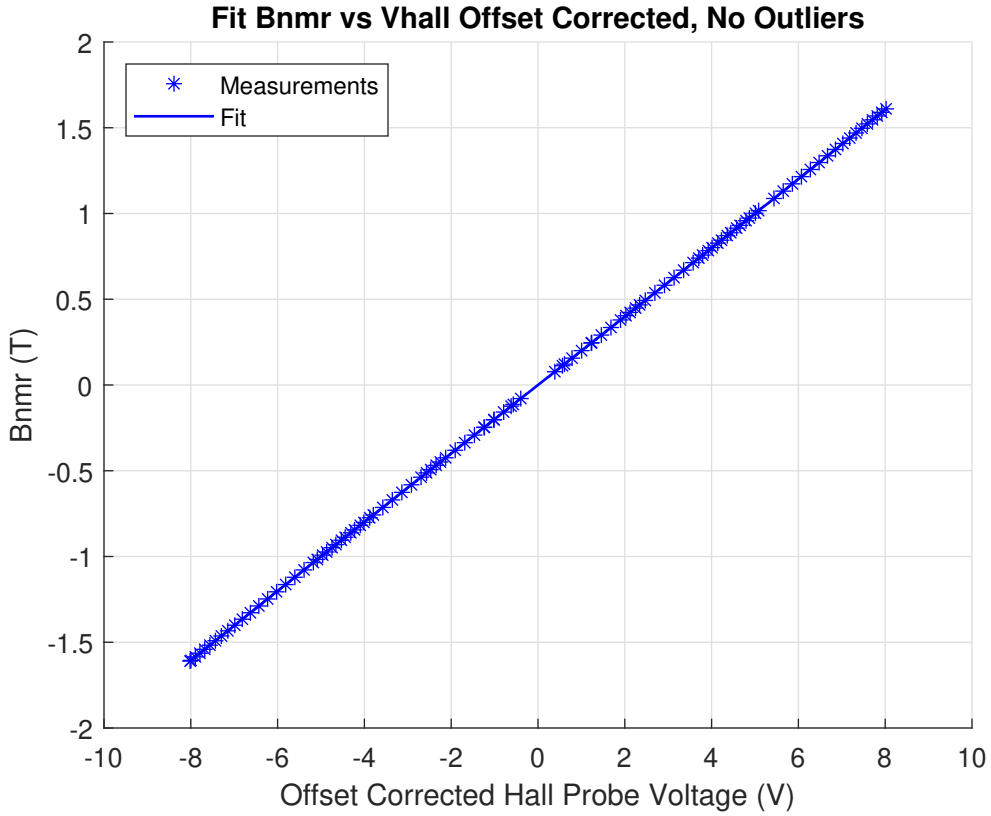
Fit Bnmr vs Vhall Offset Corrected, No Outliers
Measurements
Fit
Bnmr (T)
Offset Corrected Hall Probe Voltage (V)
2
1.5
1
0.5
0
-0.5
-1
-1.5
-2
-10
-8
-6
-4
-2
0
2
4
6
8
10

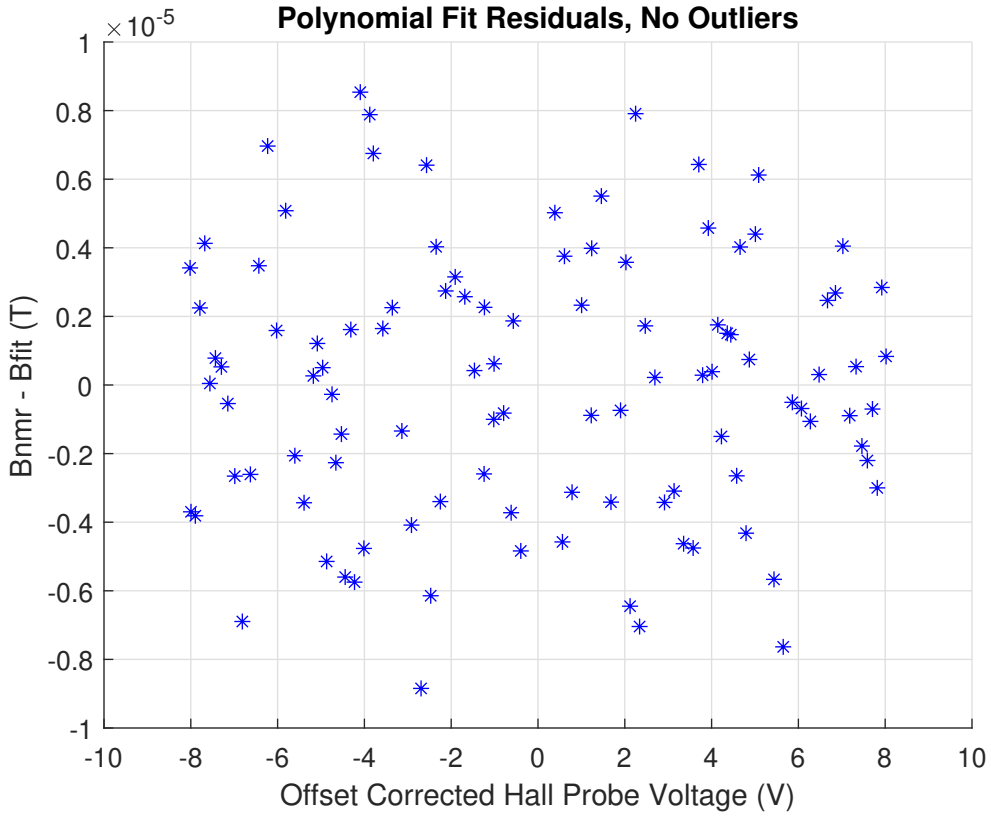
Polynomial Fit Residuals, No Outliers
×10^-5
1
0.8
0.6
0.4
0.2
0
-0.2
-0.4
-0.6
-0.8
-1
Bnmr - Bfit (T)
-10
-8
-6
-4
-2
0
2
4
6
8
10
Offset Corrected Hall Probe Voltage (V)

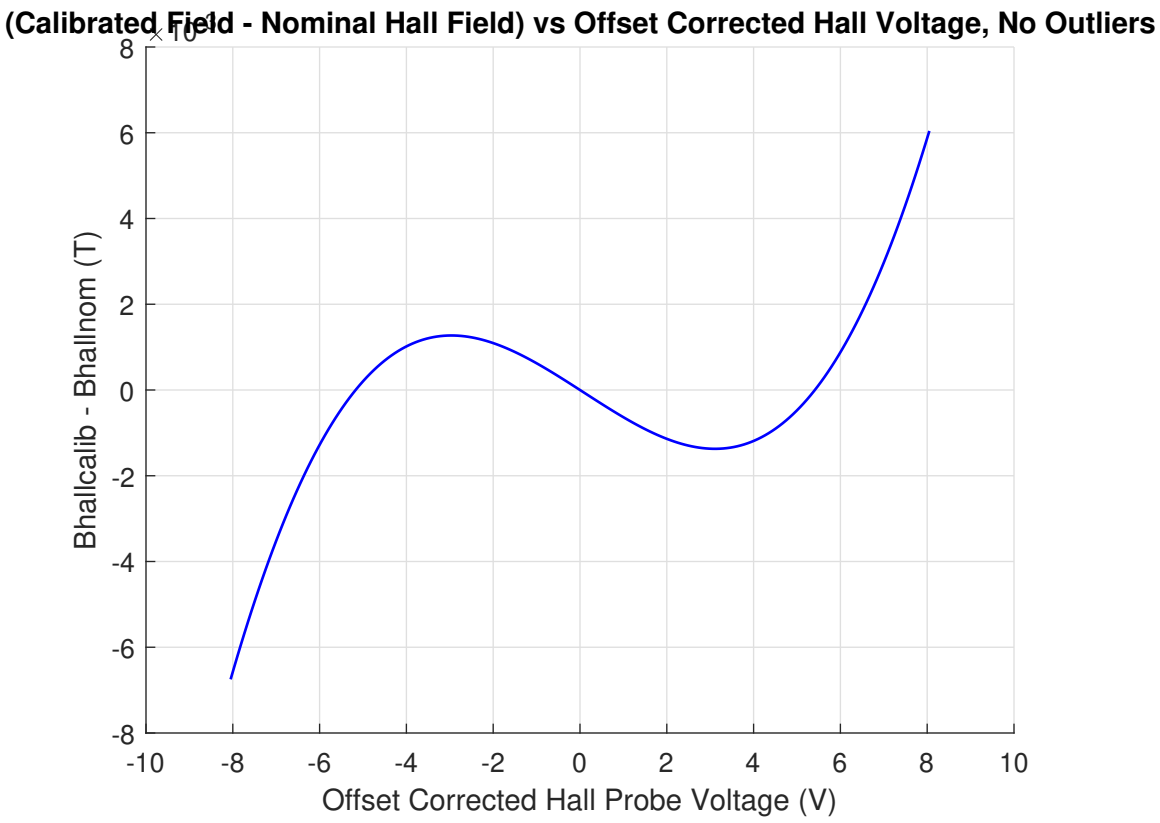
(Calibrated Field - Nominal Hall Field) vs Offset Corrected Hall Voltage, No Outliers
×10^-4
8
6
4
2
0
-2
-4
-6
-8
Bhallcalib - Bhallnom (T)
-10
-8
-6
-4
-2
0
2
4
6
8
10
Offset Corrected Hall Probe Voltage (V)